MICRON LABORATORY SERVICES

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00

9 Beatty Avenue, Witbank 1035 Tel: 013 690 1532 Fax: 013 656 1000
Postnet Suite 139 Private Bag X 7260 Witbank 1035
Reg No: 2017/365305/07 Vat nr: 4430102030
www.micronlab.co.za

CERTIFICATE OF CALIBRATION

Certificate no:	NKOT MO2.5 B
Date of calibration:	11.12.2025
Date of next calibration:	December 2026
Customer:	AzureSky (Pty) Ltd Unit 3, 17 Markiel Road Wadeville Germiston, 1401
Location:	Sample Prep
Contact:	nonhlanhla@azuresky.it.com

Conditions of Issue:

This certificate is issued in accordance with the conditions of accreditation granted by the South African National Accreditation System of South Africa. Subject to the uncertainties specified, this is a correct record of measurements made.

Copyright of this certificate is owned jointly by SANAS and the issuing laboratory. This certificate may not be reproduced other than in full without written approval of SANAS and of the issuing laboratory.

The values in this certificate were correct at the time of calibration. Subsequently the accuracy will depend on such factors as, the care of handling, the use of the instrument and the frequency of use. Re-calibrations should be performed after a period which has been chosen to ensure that the instrument's accuracy remains within the desired limits.

Where statements of conformity are made in the certificate, the following rules are applied:
Within Tolerance: Results ± expanded uncertainty within limits / specification.
Out of Tolerance: Results ± expanded uncertainty exceeds limits / specification.
Indeterminate: Results ± expanded uncertainty overlaps limits / specification.

Measurement results relate only to the item calibrated.

Technical Signatory: Z Sampson

Calibrated by: T Nchabeleng

MICRON LABORATORY SERVICES

t +27 (0)13 690 1532 | f +27 (0)13 656 1000 | e admin@mlabs.co.za | 9 Beatty Avenue, Witbank, 1035
Postnet suite 139, Private bag X7260, Witbank, 1035

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00

CERTIFICATE OF CALIBRATION

Customer:	AzureSky (Pty) Ltd	**Certificate Number:**	NKOT MO2.5 B
Contact:	nonhlanhla@azuresky.it.com	**Instrument:**	Lazzaro Oven
Location:	Sample Prep	**Serial Number:**	LZ 005/07/10
Date of Calibration:	11.12.2025	**Company Number:**	AS8501
Date of Next Calibration:	December 2026	**Procedure Reference:**	P4.1.2.HC1

Calibration Standards	**Description**	**Model**	**Coy No**	**Re-calibration date**
	OMEGA LOGGER	HH374 (V 4.3.0.0)	DL18	31st March 2026
	OMEGA LOGGER	HH378 (V 4.5.0.0)	DL19	31st March 2026
	FLEXI-PROBE x 8	OVEN	OP11	30th August 2026

Calibration Results - Before Adjustment - ºC

TOP			CENTER		BOTTOM		
39.6	38.8	39.8	38.9	38.5	39.4	39.4	38.6
DOOR			DOOR		DOOR		

The above individual readings are the average values measured at 20 second intervals over a period of 24 minutes

Calibration Results - After Adjustment - ºC

TOP			CENTER		BOTTOM		
39.6	38.8	39.8	38.9	38.5	39.4	39.4	38.6
DOOR			DOOR		DOOR		

The above individual readings are the average values measured at 20 second intervals over a period of 24 minutes

Nominal Value °C	37	**Uncertainty of Measurement ± °C**	1.1

Method: The device under test (DUT) was calibrated by comparison to the laboratory standard at the listed temperature, temperature readings were taken over a period to include deviation from set point.
Uncertainty: The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor K=2. Which for a normal distribution corresponds to a probobility of approximatley 95%. The uncertainty in the calculated uncertainty of measurement for all of the individual readings.
Traceability: The standards used for calibration are traceable to the national measuring standard.

Controller Settings	**Controller Off-Set °C**	0.0	**Note:** Adjustment to any of these controller settings will affect the unit accuracy, ramp rate and STD deviation.
	Proportional Band (P)	3	
	Integration Time (I)	100	
	Derivative Time (D)	70	
Enviromental conditions during calibration	**Temperature at start °C**	24	**± 2°C**
	Temperature at end °C	26	**± 2°C**
Remarks	**Within tolerance**		

Technical Signatory: Z Sampson

Calibrated By: T Nchabeleng

MICRON LABORATORY SERVICES


t +27 (0)13 690 1532 | f +27 (0)13 656 1000 | e admin@mlabs.co.za | 9 Beatty Avenue, Witbank, 1035
Postnet suite 139, Private bag X7260, Witbank, 1035

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00


CERTIFICATE OF CALIBRATION

Customer:	AzureSky (Pty) Ltd	**Certificate Number:**	NKOT MO2.5 B
Contact:	nonhlanhla@azuresky.it.com	**Instrument:**	Lazzaro Oven
Location:	Sample Prep	**Serial Number:**	LZ 005/07/10
Date of Calibration:	11.12.2025	**Company Number:**	AS8501
Date of Next Calibration:	December 2026	**Procedure Reference:**	P4.1.2.HC1


TOP AREA MAPPING

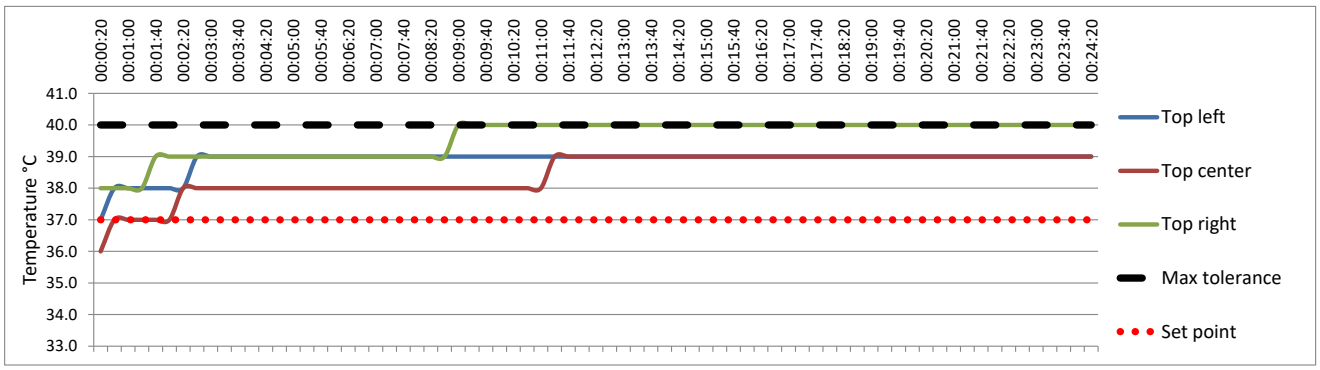

MIDDLE AREA MAPPING

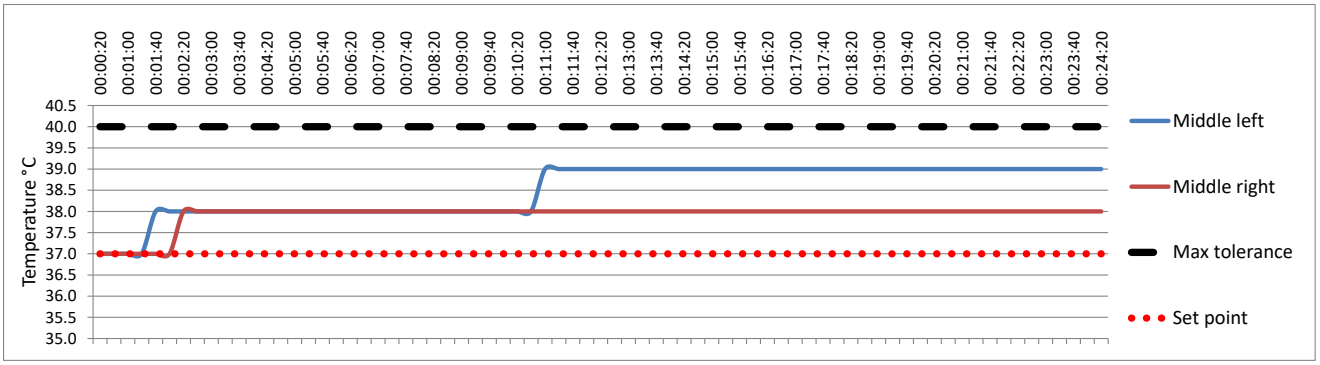

BOTTOM AREA MAPPING

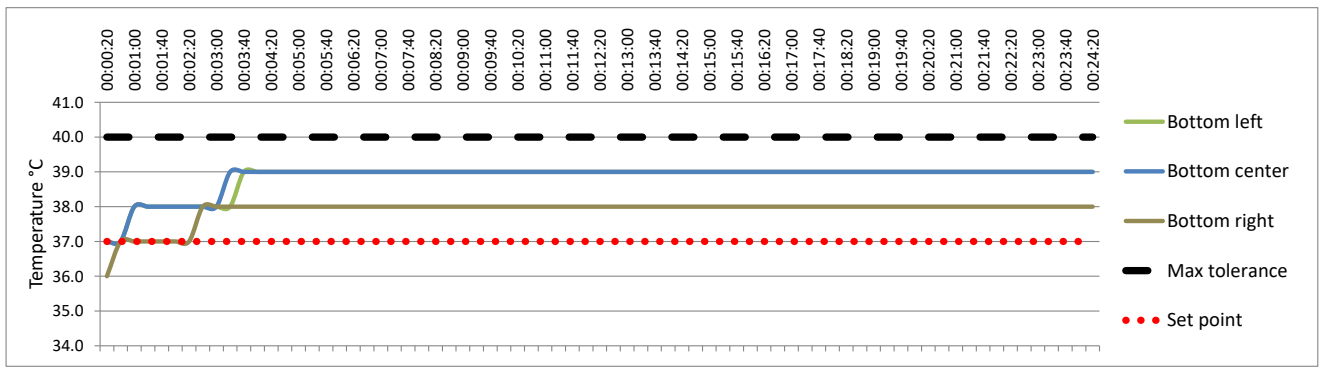

Signed by:Zelda Sampson
Signed at:2025-12-15 09:27:55 +02:00
Reason:I approve this document

Technical Signatory: Z Sampson

Calibrated By: T Nchabeleng

End Of Certificate