# SOMATOM X.cite CT5XCITIBT

Siemens Healthineers
Global Training Center

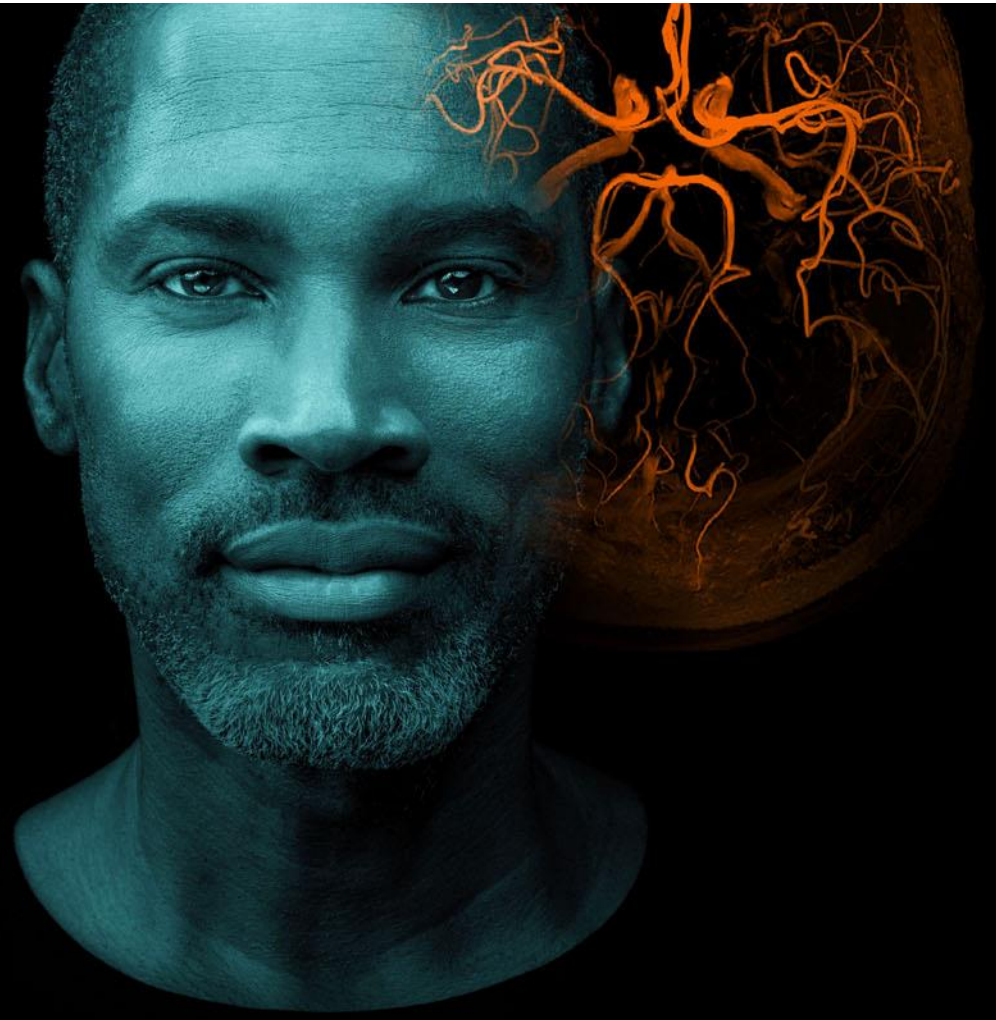

Restricted © Siemens Healthineers, 2019

SIEMENS Healthineers

# WELCOME to SOMATOM X.cite

## CT5XCITIBT

**Interactive Broadcast Training**
**SOMATOM X.cite Technical training**

CT Technical Educational Design Team
SHS CS EDU EMEA CT TEC

# Disclaimer

SIEMENS Healthineers

Please note that the learning material is for **training purposes only!**

For the proper handling of the software or hardware components, please always use the official Cloud Based Documentation and Operator Manual issued by Siemens Healthineers.

This training is meant as study material only and does not substitute the official procedures described on Cloud Based Documentation and Operator Manual.

All documents and information used in this training, are not subjected to immediate updates upon new feature release and are only referring to the software and hardware versions available during development of the training.

**Always use the newest Computer Based Documentation and Operator Manual as your main reference.**

The **reproduction, transmission or recording** of this interactive training or its contents without express written consent, it´s **NOT PERMITED**. Offenders will be held accountable according to the law.

All rights, including rights created by patent grant or registration of utility model or design, are reserved.


Restricted © Siemens Healthineers, 2019

# **CT5XCITIBT** SOMATOM X.cite Pre-Training (IBT)

SIEMENS Healthineers

**SOMATOM X.cite Pre-Training Interactive Broadcast Training**
SOMATOM X.CITE Update Training (Part 1)

**Course details**

**Target group**
CSEs that are responsible to do service and maintain a SOMATOM X.cite and further product line Systems

**Learning target**
Get information about the HW and SW features of SOMATOM X.cite

**Prerequisites**
Knowledge of Native Syngo and Definition family classroom training


Restricted © Siemens Healthineers, 2019

## SOMATOM X.CITE Pre-Training Interactive Broadcast Training

### Learning Objectives

At the end of this course, the participant should be able to recognize the functions of all different components of the system, being able to identify their locations and interconnections.

The participant should be able to assist remote troubleshooting tasks, perform defined procedures and part replacement of defined components, providing that detailed instructions are available in official documentation and part replacement is suggested by remote troubleshoot experts.

The acquired knowledge, plus the field experience should give the participant access to a second part of training, specifically focused on Hands on practice.


Restricted © Siemens Healthineers, 2019

# CT5XCITIBT Agenda

SIEMENS Healthineers

| Day | IBT Session | Approximate Time | Topics |
|---|---|---|---|
| Day 1 | 1 | 3h | Introduction of Participants<br>Course Introduction<br>X.cite Safety Instructions<br>Technical Documentation<br>CB-DOC / Function Description<br>SOMATOM X.cite Overview |
| | 2 | 3h | Power Distribution:<br>• PDS & PDB<br>• Slip Ring System<br>• Transformer<br>• UPS<br>• Switching on/off |


Restricted © Siemens Healthineers, 2019

# CT5XCITIBT Agenda

SIEMENS Healthineers

| Day | IBT Session | Approximate Time | Topics |
|---|---|---|---|
| Day 2 | 3 | 3h | Gantry Functions<br>• Rotation circuit<br>• Tilt<br>• Gantry Cooling<br>• System Firmware & Admin Portal<br>• State Diagram / Eventlog Message Domain |
| | 4 | 3h | System Control:<br>• SiDaNet<br>• Stop Circuit & Safety Circuit<br>• Internal Network<br>• GPB / Tablet / WAP<br>• Lighting<br>• 2D Camera / VPI |


Restricted © Siemens Healthineers, 2019

# CT5XCITIBT Agenda

SIEMENS Healthineers

| Day | IBT Session | Approximate Time | Topics |
|---|---|---|---|
| Day 3 | 5 | 3h | X-Ray Generator<br>• HV-Tank<br>• E-Box and P-Box<br>• Arcing Location Detection (ALD)<br>• XTA and XTC<br>• Vectron tube design and concept<br>• Tube Cooling circuit |
| | 6 | 3h | Data Measurement System<br>• Overview of DMS<br>• Data Transmission<br>• DSM & DSF<br>• Modules<br>Collimator |


Restricted © Siemens Healthineers, 2019

# CT5XCITIBT Agenda

SIEMENS Healthineers

| Day | IBT Session | Approximate Time | Topics |
|---|---|---|---|
| Day 4 | 7 | 3h | Overview of Patient Handling Systems<br>• Vario 2<br>• Vario RT<br>• Vitus |
| | 8 | 3h | ICS / IRS<br>• Overview of ICS and IRS used<br>• Remote Login IRS<br>• Spare Parts<br>• 3D Camera<br>• Software handling Overview<br>• Recovery Image<br>• Backup / Restore Functionality |


Restricted © Siemens Healthineers, 2019

# CT5XCITIBT Agenda

SIEMENS Healthineers

| Day | IBT Session | Approximate Time | Topics |
|---|---|---|---|
| Day 5 | 9 | 3h | Software and System Review |
| | 10 | 3h | Test |


Restricted © Siemens Healthineers, 2019

# Access to the Certification Test

SIEMENS Healthineers

You need to assure that you have access to your “myTraining” account on our Training Center platform.

To do so, login with your email address and your password here:

**https://www.training.healthcare.siemens.com**

In case you have forgotten your password, you can request a new one. To do this you will need access to your Siemens Healthineers e-mail account. If you do not have access to your Siemens Healthineers
e-mail account please ask your instructor for assistance.

Restricted © Siemens Healthineers, 2019

# Work on Electrical Systems

## Important Safety Instructions


Restricted © Siemens Healthineers, 2019

# Safety: Work on Electrical Systems

Before starting any installation, service or maintenance activities within the system components, switch off the system and secure the system against unintended switch-on.

The **5 safety rules** must be strictly observed.

Observing of these **5 safety rules** is essential (dangerous to life) when working on electrical systems!


Restricted © Siemens Healthineers, 2019

# 5 Safety Rules
# Must Be Strictly Observed

1. Disconnect mains!
2. Prevent reconnection!
3. Test for absence of harmful voltages!
4. Ground and short circuits!
5. Cover or close of nearby live parts!

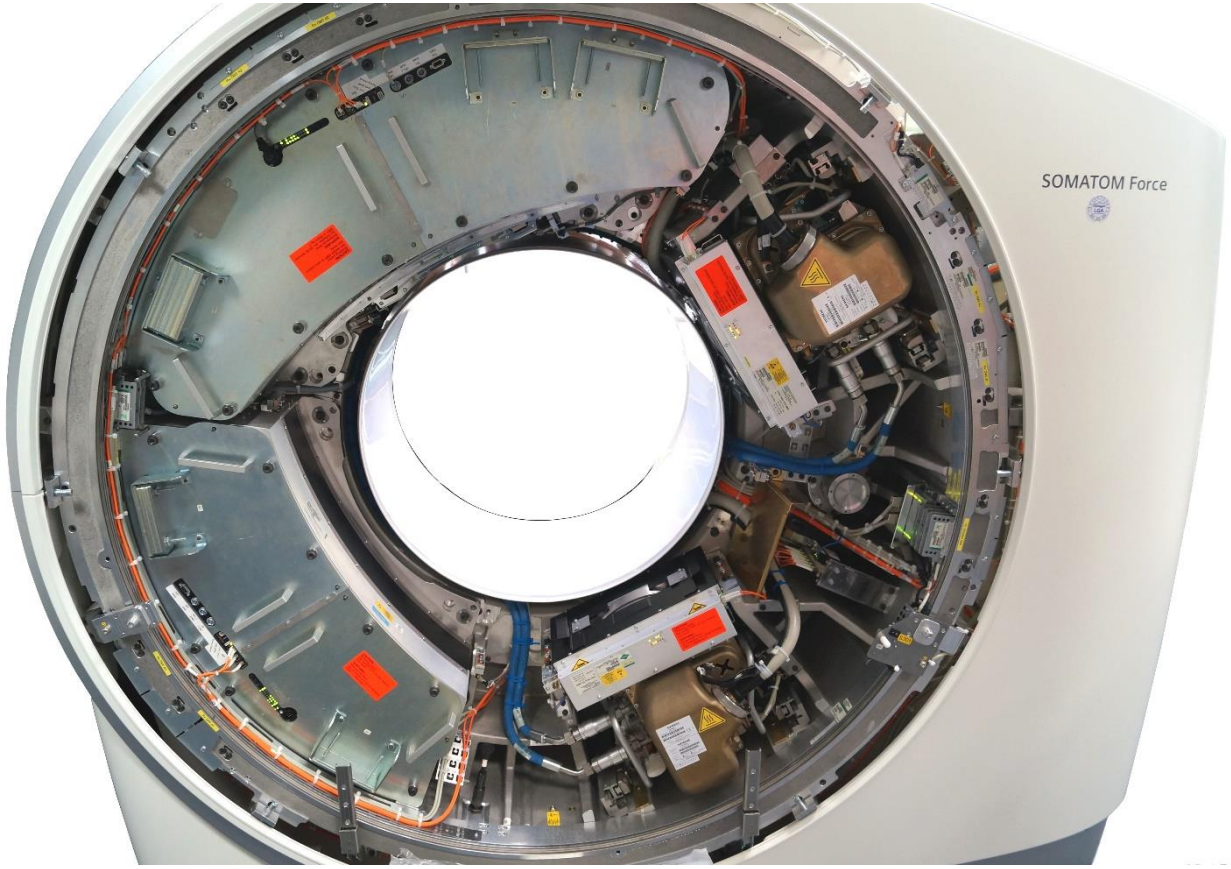



Restricted © Siemens Healthineers, 2019

# Safety: Work on Electrical Systems

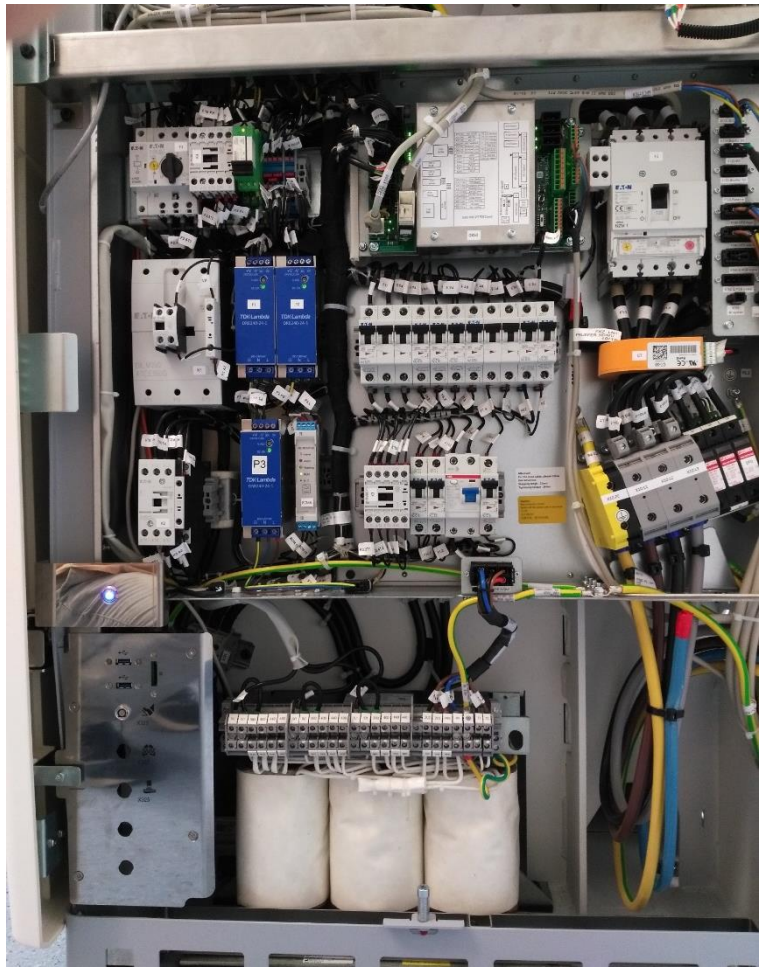

**Do not work on any parts where voltages > 25 VAC or > 60 VDC are present.**

Measurement and adjustment points have to be accessible to personnel without the risk of danger. If this is not possible, the equipment has to be shut down.

Specially dangerous components are marked with official symbol for Hazardous electrical voltage, as described on system documentation.

A waiting period might be necessary for some components to discharge any residual voltage after system shutdown.

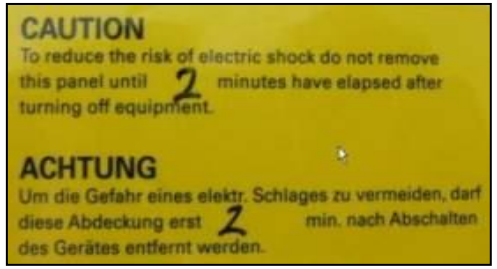



Restricted © Siemens Healthineers, 2019

# Safety: Work on Electrical Systems

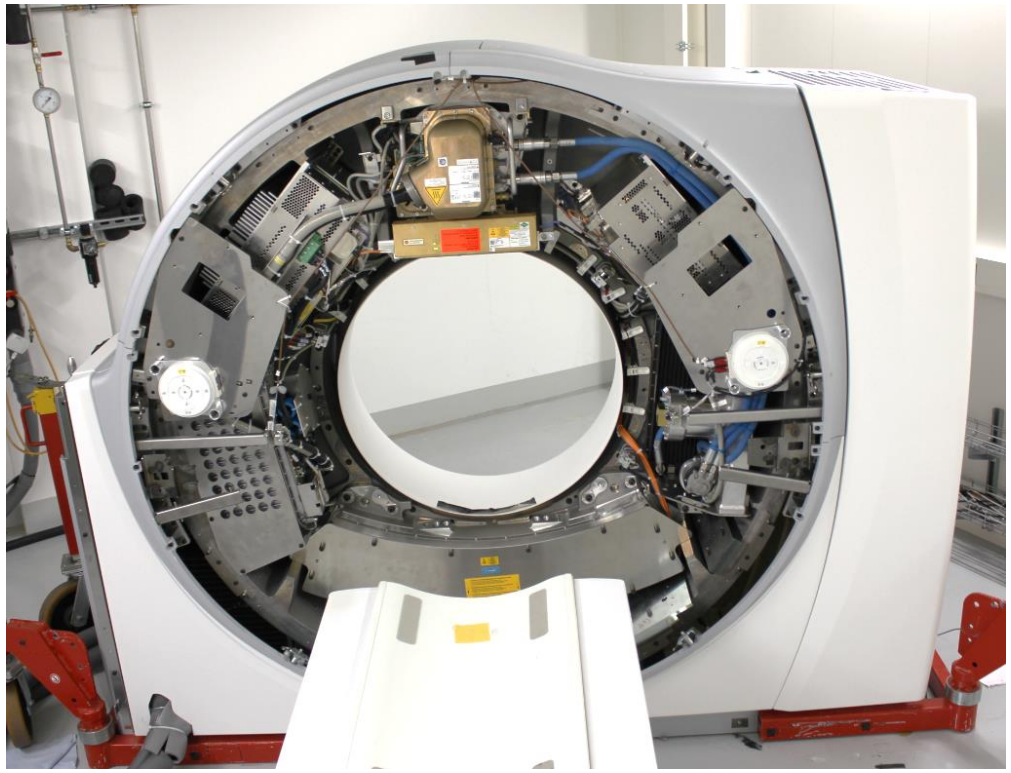

**Do not touch the power sliprings. The applied voltage could be up to 440VAC.**

**Dangerous voltages up to 150KV/DC and 440VAC are also present on other parts the System.**

Make sure that no other person can switch on power or switch off security measures, when performing installation, maintenance or service work at the system.

**Possible movements of system components**

- To avoid injury, pay attention when moving any system components.
- Wait until rotation has come to a complete stop.
- Spontaneous table movement occur during checkup


Restricted © Siemens Healthineers, 2019

# Electrical System Incident – Mains Distributor

- In case of an incident turn off the system.
- Protective covers **must not be opened**.
- Modifications to standard connections are not allowed.
- Working on mains distributors is only allowed for **electrically qualified people.**


Restricted © Siemens Healthineers, 2019

# Thank you
# for your enthusiasm!

**Siemens Healthineers**
Siemens Healthcare GmbH
CT Technical Educational Design Team
Customer Services Education
Allee am Roethelheimpark 3 A
91052 Erlangen, Germany
Fax: +49 9131 846492
trainingcenter-erlangen.team@siemens-healthineers.com


Restricted © Siemens Healthineers, 2019