Exact pairing on each assay-specific design panel
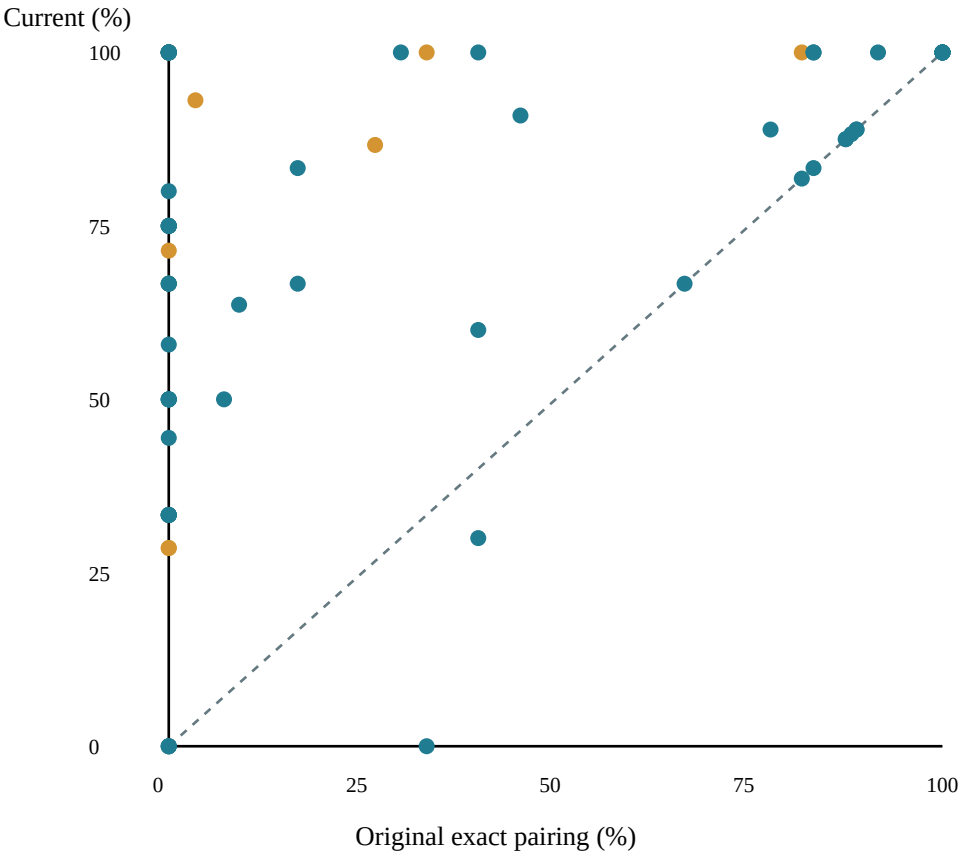
Each point is one catalog entry; both axes use the same accession set