Hotgen

COMPACT AUTOMATIC

CHEMILUMINESCENCE IMMUNOASSAY SYSTEM

Unstable Power? Reliable Operation with UPS.



MQ 60 smart



MQ 60 proB

Test Menu

Panel	Parameter	Qualification	Linear Range	Reference Values	Sample Type
Cardiac	hs-cTnT	CE IVDR	3-10000 pg/mL	<14 pg/mL	S/P/WB
	hs-cTnI	NMPA, CE IVDR	0.02-50 ng/mL	0.04 ng/mL	S/P/WB
	CK-MB	NMPA, CE IVDR	2-500 ng/mL	4.99 ng/mL	S/P/WB
	MYO	NMPA, CE IVDR	5-1000 ng/mL	48.8 ng/mL	S/P/WB
	H-FABP	NMPA, CE	0.2-300 ng/mL	10 ng/mL	S/P/WB
	Lp-PLA2	NMPA, CE	5-1000 ng/mL	200 ng/mL	S/P/WB
	NT-proBNP	NMPA, CE IVDR	50-30000 pg/mL	125 pg/mL	S/P/WB
	BNP	NMPA, CE IVDR	10-5000 pg/mL	105 pg/mL	S/P/WB
	ST2	NMPA	3-200 ng/mL	35 ng/mL	S/P/WB
	cTnI	NMPA	0.02-40 ng/mL	⩽0.04 ng/mL	S/P/WB
	D-Dimer	NMPA, CE IVDR	2.5-2500 ng/mL	350 ng/mL	P/WB
Inflammation	PCT	NMPA, CE IVDR	0.02-100 ng/mL	0.05 ng/mL	S/P/WB
	PCTm	NMPA	0.15-100 ng/mL	0.5 ng/mL	WB
	CRP	NMPA, CE IVDR	0.5-150 mg/L	For evaluation of infection: Normal CRP＜8 mg/L. For risk stratification of cardiovascular disease: Low risk: 3.0 mg/L. Medium risk: 1.0-3.0 mg/L. High risk: >3.0 mg/L.	S/P/WB
	IL-6	NMPA, CE IVDR	1.5-5000 pg/mL	7 pg/mL	S/P/WB
Tumor	CEA	NMPA, CE IVDR	0.2-1000 ng/mL	5.2 ng/mL	S/P
	CA125	NMPA, CE IVDR	0.6-5000 U/mL	35 U/mL	S/P
	HE4	NMPA, CE IVDR	15-1500 pmol/L	105 pmol/L	S/P
	CYFRA21-1	NMPA, CE IVDR	0.1-500 ng/mL	3.3 ng/mL	S/P
	CA15-3	NMPA, CE IVDR	1-300 U/mL	26.4 U/mL	S/P
	CA242	NMPA, CE IVDR	0.5-200 IU/mL	10 IU/mL	S
	CA19-9	NMPA, CE IVDR	0.6-1000 U/mL	27 U/mL	S/P
	CA72-4	NMPA, CE IVDR	0.2-300 U/mL	6.9 U/mL	S/P
	CA50	NMPA	1-500 U/mL	25 U/mL	S/P
	NSE	NMPA, CE IVDR	0.1-300 ng/mL	16.3 ng/mL	S
	proGRP	NMPA, CE IVDR	3-2300 pg/mL	63 pg/mL	S/P
	SCCA	NMPA, CE IVDR	0.1-45 ng/mL	2.3 ng/mL	S/P
	tPSA	NMPA, CE IVDR	0.1-100 ng/mL	4 ng/mL	S/P
	VEGF	NMPA	50-3200 pg/mL	⩽160 pg/mL	S
	fPSA	NMPA, CE	0.01-30 ng/mL	⩽1.2 ng/mL	S
	TK1	NMPA	1.5-20 pM	⩽2.02 pM	S/P
Liver Disease	AFP	NMPA, CE IVDR	0.6-1200 ng/mL	7 ng/mL	S/P
	AFP-L3%	NMPA, CE	5%-50%	<10%	S/P
	DCP	NMPA, CE	5-20000 ng/mL	40 ng/mL	S
	GP73	NMPA, CE	50-500 ng/mL	150 ng/mL	S/P
	CK18-M30	NMPA	Qualitative	200 U/L	S
	CK18-M65	NMPA	Qualitative	460 U/L	S
Gastric Function	G-17	NMPA, CE IVDR	20-1000 pg/mL	<43.68 pg/mL	S/P
	PGI	NMPA, CE IVDR	1-200 ng/mL	70 ng/mL. The reference value of PG I/PG II ratio in normal samples was above 3 when PG I and PG II combined detection was performed.	S/P
	PGII	NMPA, CE IVDR	0.5-100 ng/mL	<23.85 ng/mL. The reference value of PG I/PG II ratio in normal samples was above 3 when PG I and PG II combined detection was performed.	S/P
	H. pylori Ab	NMPA	Qualitative	1.0 COI	S/P
	H. pylori Urease Ab	/	Qualitative	1.0 COI	S/P
Renal Function	NGAL	NMPA, CE	10-1000 ng/mL	145 ng/mL	S/Urine
	CysC	NMPA, CE	0.02-4 mg/L	1.2 mg/L	S/P/WB
	Anti-PLA2R	NMPA	6-1500 RU/mL	＜20.00 RU/mL	S/P
Anemia	Ferritin	NMPA, CE IVDR	0.5-2000 ng/mL	Male: 30-400 ng/mL; Female: 13-150 ng/mL.	S/P
	VB12	NMPA, CE IVDR	100-1800 pg/mL	190 pg/mL-910 pg/mL	S/P
	FA	NMPA, CE IVDR	1.0-24.0 ng/mL	3.5-20 ng/mL	S/P

Test Menu

Panel	Parameter	Qualification	Linear Range	Reference Values	Sample Type
Thyroid	TSH	NMPA, CE IVDR	0.1-100 mIU/L	0.27 mIU/L-4.2 mIU/L	S/P
	TT4	NMPA, CE IVDR	10-240 ng/mL	51-141 ng/mL	S/P
	TT3	NMPA, CE IVDR	0.25-6.0 ng/mL	0.8-2.0 ng/mL	S/P
	FT4	NMPA, CE IVDR	1.0-76 pg/mL	9.3 pg/mL-17 pg/mL	S/P
	FT3	NMPA, CE IVDR	0.95-32 pg/mL	2.0 pg/mL-4.4 pg/mL	S/P
	Anti-TG	NMPA, CE IVDR	15-4000 IU/mL	115 IU/mL	S/P
	Anti-TPO	NMPA, CE IVDR	5.0-600 IU/mL	34 IU/mL	S/P
Immuog -lobulins	IgE	CE	0.5-1500 IU/mL	Age group: New born: <1.5 IU/mL; 1-12 months: <15 IU/mL; 1-5 years old: <60 IU/mL; 6-9 years old: <90 IU/mL; 10-15 years old:<200 IU/mL; Adult: <100 IU/mL.	S/P
Sex hormone	FSH	NMPA, CE IVDR	0.5-200 IU/L	Male: 1.5-12.3 IU/L; Female: Follicular phase: 3.5-12.5 IU/L; Ovulation phase: 4.7-21.5 IU/L; Luteal phase: 1.7-7.7 IU/L; After menopause: 25.8-134.5 IU/L;	S/P
	E2 (Estradiol)	NMPA, CE IVDR	10-3000 pg/mL	Male: 25.1-60.5 pg/mL; Female: Follicular phase: 12.3-233 pg/mL; Ovulation phase: 41-398 pg/mL; Luteal phase: 22.5-341 pg/mL; After menopause: <10-138 pg/mL; Pregnancy early phase: 155->3000 pg/mL.	S/P
	TESTOSTERONE	NMPA, CE IVDR	0.10-15 ng/mL	Male: 1.93-8.36 ng/mL; Female: 0.10-0.48 ng/mL.	S/P
	PROGESTERONE	NMPA, CE IVDR	0.10-50 ng/mL	Male: 0.2-1.4 ng/mL; Female: Follicular phase: 0.2-1.5 ng/mL; Ovulation phase: 0.8-3.0 ng/mL; Luteal phase: 1.7-27 ng/mL; After menopause: 0.1-0.8 mL.	S/P
	LH	NMPA, CE IVDR	1.0-200 IU/L	Male: 1.7-8.6 IU/L; Female: Follicular phase: 2.3-12.5 IU/L; Ovulation phase: 14.0-95.0 IU/L; Luteal phase: 1.1-11.4 IU/L; After menopause: 7.7-58.5 IU/L.	S/P
	PRL (PROLACTIN)	NMPA, CE IVDR	5.0-5000 mIU/L	Male: 55-325 mIU/L; Female (Non-pregnant): 101-495 mIU/L.	S/P
	AMH	NMPA, CE IVDR	0.05-23 ng/mL	Female: Age group: 20-39: 0.5-9.95 ng/mL; 40-50: 0.05-4.44 ng/mL.	S/P
	β-HCG	NMPA, CE IVDR	2-15000 mIU/mL	Non-pregnant women: 5.2 mIU/mL; Pregnant women: 1-10 weeks: 200-230080 mIU/mL; 11-15 weeks: 22540-234900 mIU/mL; 16-22 weeks: 8050-50100 mIU/mL; 23-40 weeks: 1620-49445 mIU/mL.	S/P
	Inhibin B	CE	10-1300 pg/mL	Male: 18.42-270.30 pg/mL; Female: Age group： 20-50: 14.25-97.53 pg/mL; >50: <10-13.27 pg/mL.	/
Growth Hormone	G. HORMONE	NMPA, CE IVDR	0.06-40 ng/mL	Male: Age group: 1-10: 0.097-6.27 ng/mL; 11-18: 0.081-10.76 ng/mL; 19-79: 0.041-2.41 ng/mL; Female: Age group: 1-10: 0.118-7.78 ng/mL; 11-18: 0.128-8.00 ng/mL; 19-77: 0.128-9.85 ng/mL.	S/P
	IGFBP-3	NMPA, CE IVDR	0.1-16 μg/mL	Age group: 1-6: 0.726-5.17 μg/mL; 7-10: 1.47-7.22 μg/mL; 11-18: 2.9-8.99 μg/mL; 19-64: 3.09-7.56 μg/mL; 65-80: 2.89-5.62 μg/mL.	S/P
	IGF-1	/	/	/	/
Diabetes	HbA1c	NMPA, CE IVDR	4%-16%	4.0%-6.0%	WB
	C-P	NMPA, CE	0.01-40 ng/mL	1.02-4.31 ng/mL	S/P
	INS	NMPA, CE	0.2-1000 μIU/mL	2.16-25.1 μIU/mL	S/P
	ADP	NMPA	0.1-60 μg/mL	0.92 μg/mL-13.51 μg/mL	S/P
	GADA	NMPA, CE IVDR	5-250 IU/mL	10 IU/mL	S/P
	IA-2A	NMPA, CE IVDR	5-250 IU/mL	10 IU/mL	S/P
	IAA	NMPA, CE IVDR	Qualitative	1.0 COI	S/P
	ICA	NMPA, CE IVDR	Qualitative	1.0 COI	S/P
Hypertension	Cortisol	NMPA, CE	0.4-60 μg/dL	Morning: 6.6-23.1 μg/dL; Afternoon: 10.3 μg/dL	S/P/Urine
	ALD	NMPA, CE	20-1000 pg/mL	Standing position: 70-300 pg/mL; Lying down position: 30-160 pg/mL.	S/P
	Renin	NMPA, CE	0.5-500 pg/mL	Standing position: 2.8-28.4 pg/mL; Lying down position: 1.9-24.5 pg/mL.	P
	ACTH	NMPA	1-2000 pg/mL	7.20-63.5 pg/mL	P
Bone Metabolism	25-OH-VD	NMPA, CE IVDR	3-120 ng/mL	30-150 ng/mL	S/P
	PTH	NMPA, CE	5.5-2300 pg/mL	14.28-56.15 pg/mL	S/P
	BGP	NMPA, CE	0.5-300 ng/mL	Healthy male: Age group： 18-<30: 24.05-70.21 ng/mL; 30-50: 14.22-42.05 ng/mL; ＞50-70: 14.30-46.03 ng/mL; Female: Healthy female: Premenopausal: 11.17-43.12 ng/mL; Postmenopausal: 15.09-46.23 ng/mL; Patients with osteoporosis: 13.21-48.02 ng/mL.	S/P
	Total P1NP	NMPA	5-1200 ng/mL	Premenopausal women: 15.25-58.83 ng/mL; Postmenopausal women: 16.12-73.17 ng/mL.	S/P
	β-CTx	NMPA	0.01-6 ng/mL	Male: Age group: 30-50: 0.585 ng/mL; ＞50-70: 0.711 ng/mL; ＞70: 0.859 ng/mL; Female: Premenopausal: 0.576 ng/mL; Postmenopausal: 1.042 ng/mL.	S/P
Brain Injury	S100	NMPA	0.02-30 ng/mL	0.105 ng/mL	S


Test Menu

Panel	Parameter	Qualification	Linear Range	Reference Values	Sample Type
Rheumatoid Arthritis	Anti-CCP	NMPA, CE IVDR	10-500 U/mL	⩽17.30 U/mL	S/P
	RF-IgA	NMPA	2-200 RU/mL	＜20 RU/mL	S/P
	RF-IgM	NMPA	2-200 RU/mL	＜20 RU/mL	S/P
	RF-IgG	NMPA	2-200 RU/mL	＜20 RU/mL	S/P
Cytokine	IL-2	NMPA, CE	2.5-1000 pg/mL	12 pg/mL	S
	IL-4	NMPA	2.5-2500 pg/mL	12.8 pg/mL	S/P
	IL-5	NMPA	2.5-2500 pg/mL	5.9 pg/mL	S
	IL-8	NMPA, CE	5-7500 pg/mL	63 pg/mL	S
	IL-10	NMPA, CE	3-1000 pg/mL	9.5 pg/mL	S
Cytokine	IL-1β	NMPA, CE	3-1000 pg/mL	4.9 pg/mL	S
	TNFα	NMPA, CE	3-1000 pg/mL	8.5 pg/mL	S
	IL-2R	NMPA,CE IVDR	5-7500 U/mL	228-724 U/mL.	S/P
	IL-17A	NMPA	2.5-2500 pg/mL	5.6 pg/mL	S/P
	IFN- γ	NMPA, CE	2-1000 IU/mL	4 IU/mL	S/P
	IL-12p70	NMPA	2.5-1000 pg/mL	10.5 pg/mL	S
	IL-22	NMPA	1-1000 pg/mL	3.71 pg/mL	S
TORCH	Toxo-IgG	/	Qualitative	1.0 COI	S/P
	Toxo-IgM	/	Qualitative	1.0 COI	S/P
	RUB-IgG	/	Qualitative	1.0 COI	S/P
	RUB-IgM	/	Qualitative	1.0 COI	S/P
	CMV-IgG	/	Qualitative	1.0 COI	S/P
	CMV-IgM	/	Qualitative	1.0 COI	S/P
	HSV-1/2 IgG	/	Qualitative	1.0 COI	S/P
	HSV-1/2 IgM	/	Qualitative	1.0 COI	S/P
	HSV-1 IgG	/	Qualitative	1.0 COI	S/P
	HSV-1 IgM	/	Qualitative	1.0 COI	S/P
	HSV-2 IgG	/	Qualitative	1.0 COI	S/P
	HSV-2 IgM	/	Qualitative	1.0 COI	S/P
STAT	PCT STAT	NMPA	0.02-100 ng/mL	⩽ 0.05 ng/mL	S/P/WB
	H-FABP STAT	NMPA	0.2-120 ng/mL	⩽8.3 ng/mL	S/P/WB
	NGAL STAT	NMPA	10-1000 ng/mL	⩽145 ng/mL	S
	MYO STAT	NMPA	5-1000 ng/mL	⩽48.8 ng/mL	S/P/WB
	BNP STAT	NMPA	10-5000 pg/mL	⩽ 105 pg/mL	P/WB
	IL-6 STAT	NMPA	1.5-5000 pg/mL	⩽7 pg/mL	S/P/WB
	D-Dimer STAT	NMPA	50-10000 ng/mL	⩽500 ng/mL	P/WB
	NT-proBNP STAT	NMPA	30-30000 pg/mL	Age group: 1-18: 263.8 pg/mL; 19-49: 125.0 pg/mL; 50-75: 275.8 pg/mL; ＞75: 582.9 pg/mL.	S/P/WB
	hs-cTnI STAT	NMPA	0.02-40 ng/mL	⩽0.04 ng/mL	S/P/WB
	CK-MB STAT	NMPA	2-400 ng/mL	⩽4.99 ng/mL	S/P/WB
Infectious Disease	HBsAg	/	0.05-150 IU/mL	0.1 IU/mL	S/P
	HCV-Ab	/	Qualitative	1.0 COI	S/P
	HIV-Ab/Ag	/	Qualitative	1.0 COI	S/P
	TP-Ab	/	Qualitative	1.0 COI	S/P
Tuberculosis (TB-IGRA)	Protein extraction reagent	NMPA, CE IVDR	/	/	WB
	IFN-γ	NMPA, CE	2-1000 IU/mL	4 IU/mL	S/P

Available Coming soon

Beijing Hotgen Biotech Co.,Ltd
Add.: No.55, Qingfeng West Road, Daxing District, Beijing, 102629, P.R. China
Tel: +86 010-50986588 Website: www.hotgenbiotech.com E-mail:sales@hotgen.com.cn

MQ60 series mono-test automatic chemiluminescence immunoassay analyzers adopt chemiluminescence enzyme immunoassay technology with magnetic particle technology, through detecting the analyte substrate luminous intensity, to calculate the analyte concentration.

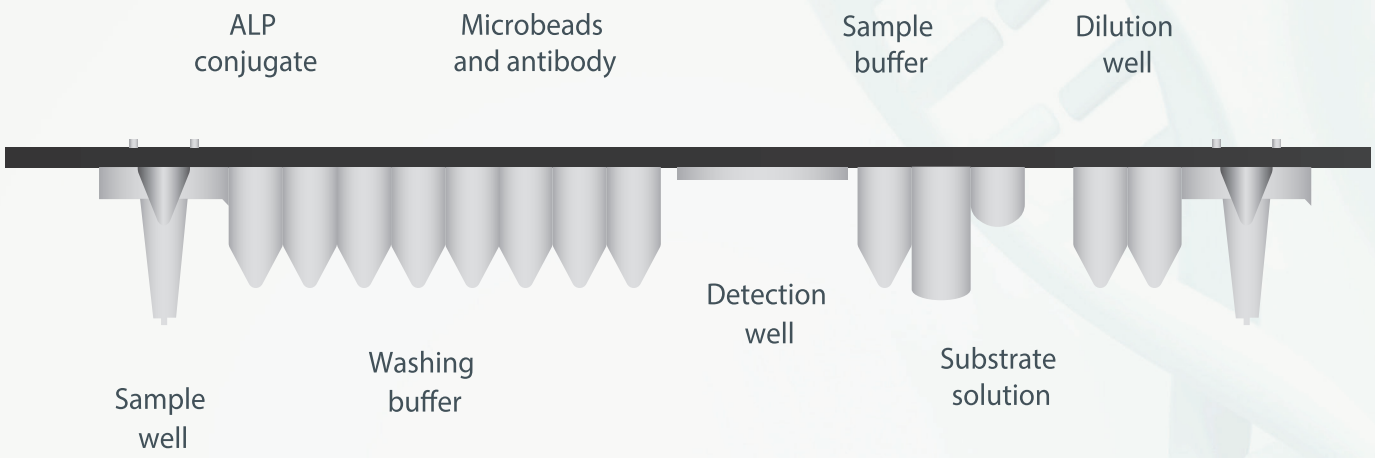

PRECISE

ALP-AMPPD magnetic particle chemiluminescence
Multiple quality controls available
CV batch-to-batch ⩽5%

FLEXIBLE

Free parameters combination
Standalone testing units

ECONOMY

Single cartridge, no hidden cost
No liquid circuit, limited maintenance

COMPACT

Compact design suitable for small to large laboratories, clinical departments
Diverse parameters covering cardiac diseases, tumor markers, fertility, thyroid, etc.

USER-FRIENDLY

Large touch screen
Fully automated, simple steps for operation

INTEGRATED UPS (OPTIONAL)

Ensures uninterrupted operation during power outages.

Application

HOSPITAL LABORATORY

LABORATORY

Technical Specifications



MQ 60 smart

Analyzer Type	Fully automated Bench-top CLIA analyzer (MQ60 smart)
Sample type	Human serum, plasma, whole blood, urine
Host size	300mm x 565mm x 610mm (length×width×height)
Host weight	36.0kg
Display	10.1 inch touch screen
Languages	English
Mode	Batch mode
Channel	6 channels
Throughput	24 tests/hour
Power supply	Voltage: AC 100-240V～
Temperature control of incubation module	Temperature stability: 37°C ± 0.5°C Temperature fluctuation: not more than 0.5°C
PC	Integrated
Printer	Internal thermal printer
Storage	Result storage >1 million
Standby	24 hours operation standby
Data management	LIS/HIS connection

Analyzer Type	Fully automated Bench-top CLIA analyzer(MQ60 proB)
Sample type	Human serum, plasma, whole blood, urine
Host size	660mm x 750mm x 600mm (length×width×height)
Host weight	80.0kg
Display	13.3 inch touch screen
Languages	English
Mode	Batch mode, STAT mode
Channel	2 modules, 12 channels
Throughput	48 tests/hour
Power supply	Voltage: AC 100-240V～
Temperature control of incubation module	Temperature stability: 37°C ± 0.5°C Temperature fluctuation: not more than 0.5°C
PC	Integrated
Printer	Internal thermal printer
Storage	Result storage >10 million
Standby	24 hours operation standby
Data management	LIS/HIS connection



MQ 60 proB