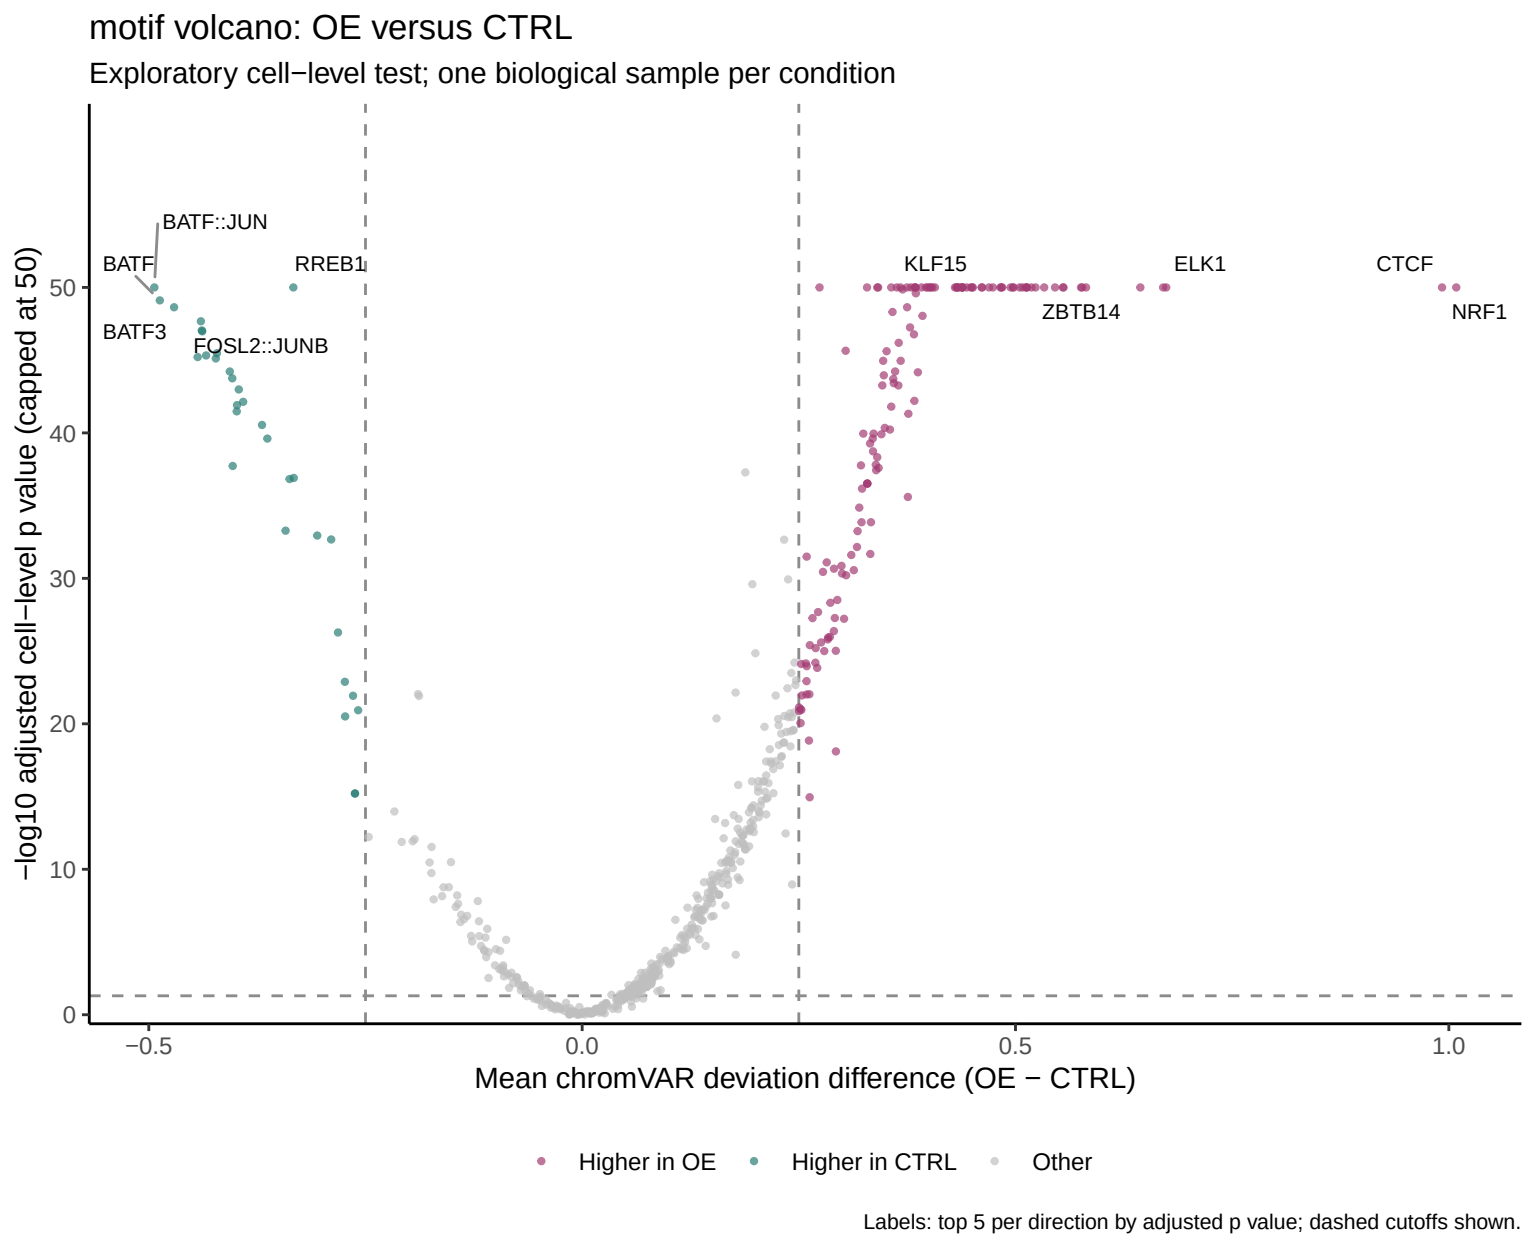
motif volcano: OE versus CTRL
Exploratory cell−level test; one biological sample per condition
BATF::JUN
BATF
RREB1
BATF3
FOSL2::JUNB
KLF15
ELK1
CTCF
ZBTB14
NRF1
−log10 adjusted cell−level p value (capped at 50)
0
10
20
30
40
50
−0.5
0.0
0.5
1.0
Mean chromVAR deviation difference (OE − CTRL)
Higher in OE
Higher in CTRL
Other
Labels: top 5 per direction by adjusted p value; dashed cutoffs shown.