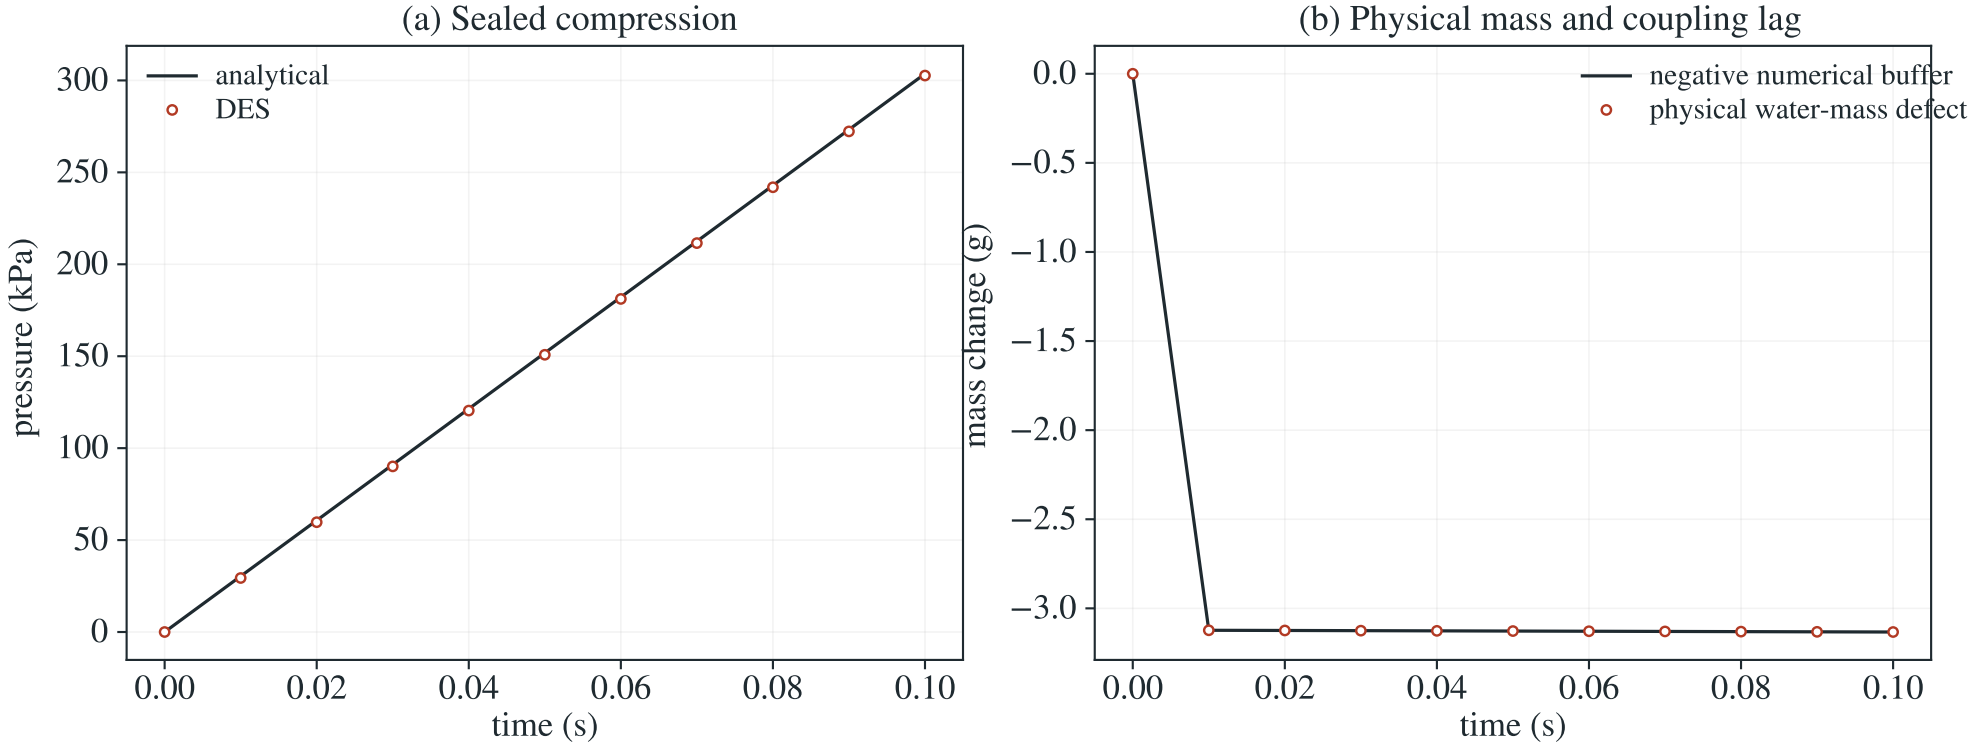

(a) Sealed compression
analytical
DES
pressure (kPa)
time (s)
0
50
100
150
200
250
300
0.00
0.02
0.04
0.06
0.08
0.10
(b) Physical mass and coupling lag
negative numerical buffer
physical water-mass defect
mass change (g)
time (s)
0.0
−0.5
−1.0
−1.5
−2.0
−2.5
−3.0