


Sample Name: AC 290 POL F-1

```
=====
Acq. Operator   : ISC                      Seq. Line :    1
Acq. Instrument : Instrument 1             Location  : Vial 1
Injection Date  : 3/12/2024 2:03:02 PM    Inj       :    1
                                           Inj Volume: 10.0 µl

Sequence File   : C:\CHEM32\1\SEQUENCE\240312.S
Method          : C:\CHEM32\1\METHODS\UHPLC.M
Last changed    : 1/6/2020 1:31:40 PM by RAS
Method Info     : UHPLC
=====
```

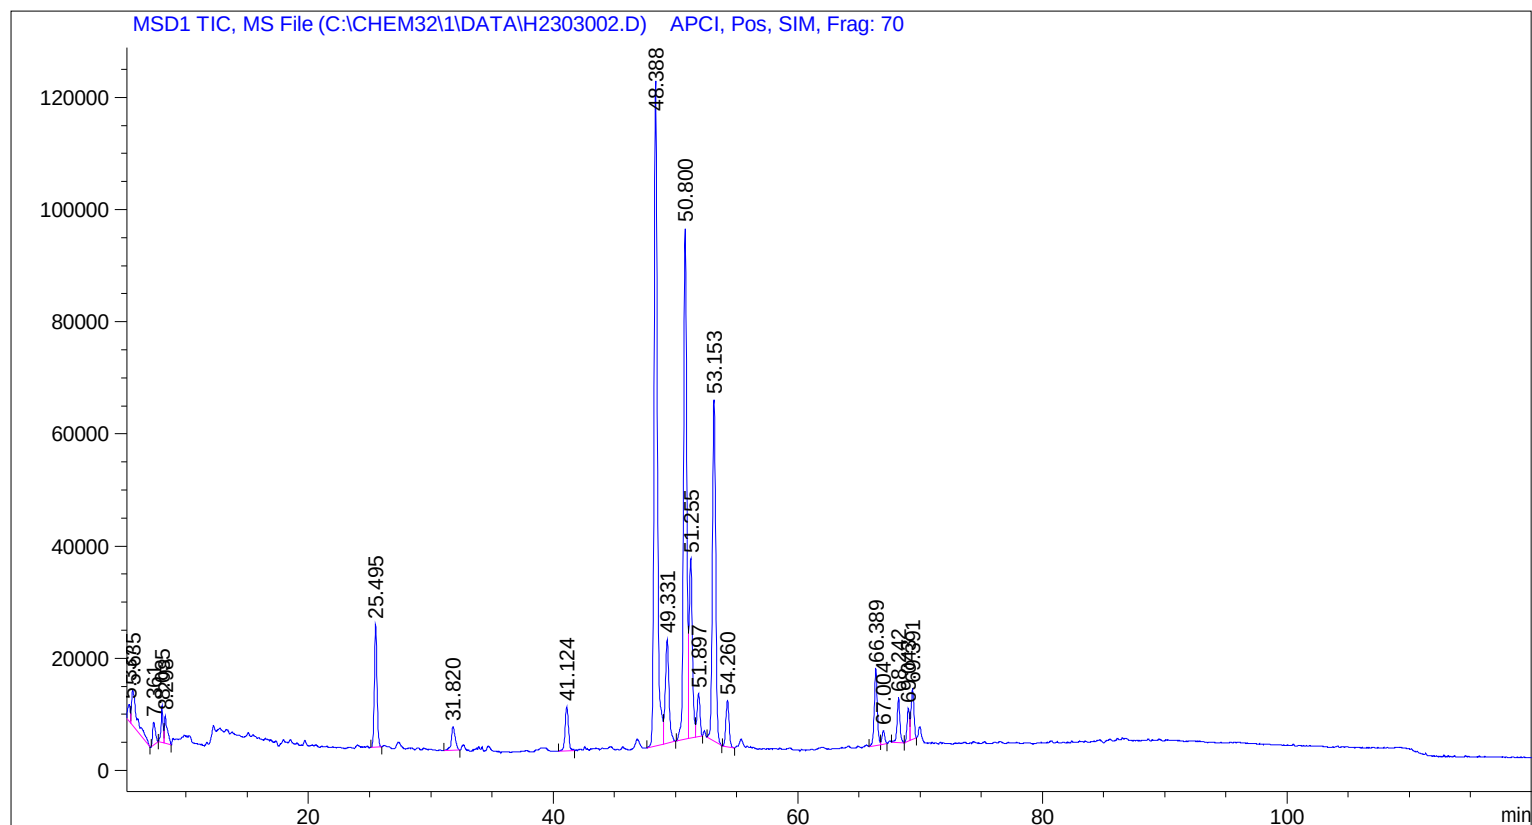

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: MSD1 TIC, MS File

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	5.337	BV	0.1954	4.05462e4	2981.24805	0.5115
2	5.635	VB	0.4696	2.01937e5	6234.19336	2.5473
3	7.361	BB	0.2535	6.41575e4	4019.75220	0.8093
4	8.035	BV	0.1637	7.18685e4	6601.26563	0.9066
5	8.298	VB	0.2331	8.40180e4	4838.90527	1.0598
6	25.495	BB	0.2306	3.29566e5	2.18965e4	4.1573
7	31.820	BB	0.3351	9.51811e4	4145.19189	1.2006
8	41.124	BB	0.3029	1.49754e5	7821.02246	1.8890

Sample Name: AC 290 POL F-1

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
9	48.388	BV	0.2854	2.21747e6	1.18594e5	27.9719
10	49.331	VB	0.3290	3.95260e5	1.84841e4	4.9859
11	50.800	BV	0.2796	1.66143e6	9.12885e4	20.9578
12	51.255	VV	0.2760	5.90124e5	3.20480e4	7.4440
13	51.897	VB	0.2667	1.31318e5	7682.77441	1.6565
14	53.153	BB	0.2942	1.12034e6	6.08832e4	14.1323
15	54.260	BB	0.2764	1.47716e5	8240.61816	1.8633
16	66.389	BV	0.2587	2.31543e5	1.36767e4	2.9208
17	67.004	VB	0.2429	3.65444e4	2345.74878	0.4610
18	68.242	BB	0.2383	1.26487e5	8049.90869	1.5955
19	69.043	BV	0.2096	8.13757e4	5906.91992	1.0265
20	69.391	VB	0.2497	1.50857e5	9038.69434	1.9030

Totals : 7.92749e6 4.34777e5

=====
*** End of Report ***