



Certificate of Calibration

Everett Service Center

Certificate Number: EVL1035363**Status:** AS-LEFT**Date of Calibration:** 01 Mar 2025**Date Due:** 01 Mar 2028**Manufacturer:** Fluke**Temperature:** 22.5 °C**Model:** 8508A**Relative Humidity:** 44.6 %**Serial Number:** 276568089**Issue Date:** 02 Mar 2025**Option(s):** 01**Description:** Reference Multimeter**Procedure:** Fluke 8508A ACAL/ZCAL VER 5720A/5725A

Rev 20231205

Customer: MODERN SURVEYING CALIBRATION & TESTING LABS(FZE)**Location:** ERBIL

IQ


PO Number: PO1250001**RMA/SO Number:** 33009838

This calibration is traceable to the International System of Units (SI) through recognized national metrology institutes (NIST, NRC, PTB, NPL, etc.), radiometric techniques, or natural physical constants and is in conformance with ISO/IEC 17025:2017. Calibration certificates without identification of the authorizing person are not valid. This certificate applies to only the item identified and shall not be reproduced except in full, without the specific written approval by Fluke Corporation.


The calibration interval (date due) is the responsibility of the end user.

This certificate of calibration may contain data that is not covered by the Scope of Accreditation. The unaccredited measurement points are indicated by the # symbol or confined to clearly marked sections. Functional (Pass / Fail) tests are not accredited.

Measurement uncertainties at the time of calibration are given where applicable. They are calculated in accordance with the method described in the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 % and $k=2$.

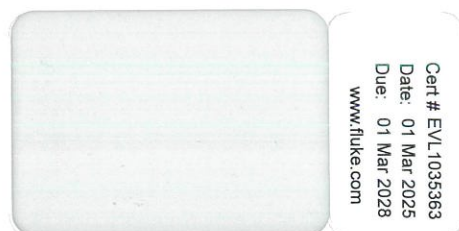

Authorized By
John Nguyen
Calibration Technician

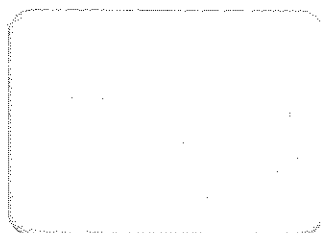

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

This calibration has been completed in accordance with:
 The Fluke Corporate Quality Manual, Revision 129
 The Fluke 17025 Quality Manual, Revision 009

This certificate does not make statements of conformity.

The following describes the symbols found in the data tables that follow:
 No symbol: Measurement value is less than or equal to the specification.
 MV>SPEC : Measurement value is greater than the specification.
 # : Out of accredited scope

Standards Used

Asset	Description	Cal Date	Cal Due
J292	Fluke 5720A Calibrator	03 Feb 2025	03 Feb 2026
J292S	Fluke 5720A / 5725A Characterized Set	05 Feb 2025	05 Mar 2025
J142	Fluke 5725A Amplifier	30 Jan 2025	30 Jan 2026
20851	Fluke 85X8A-100M 100 MOhm Resistance Standard	02 Feb 2025	02 Mar 2025
20857	Fluke 910R GPS Frequency Standard	31 Jan 2025	31 Jan 2026
J1675	Measurements International 9331G/1G Standard Resistor	12 Apr 2024	12 Apr 2025
15659	Ohm-Labs 110 10 GOhm High Resistance Standard	17 Jul 2024	17 Jul 2025
13756	Stanford Research Systems DS345 Synthesized Function Generator	22 Oct 2024	22 Oct 2025

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
Lower Limit						
Upper Limit						
8508A 1 Year Verification (99% Specification)						
UUT Firmware Version : 03.05						
Normal Ohms Verification						
2 Ohm Range (4W)						
1.0000000 Ohm	0.99975691 Ω	0.9997611 Ω	8.1 μΩ/Ω	0.9997329 Ω	0.9997809 Ω	
20 Ohm Range (4W)						
10.000000 Ohm	9.9999336 Ω	9.999919 Ω	2.5 μΩ/Ω	9.999801 Ω	10.000067 Ω	
200 Ohm Range (4W)						
100.00000 Ohm	100.002138 Ω	100.00211 Ω	2.4 μΩ/Ω	100.00113 Ω	100.00315 Ω	
2 kOhm Range (4W)						
1.0000000 kOhm	1.00000494 kΩ	1.0000043 kΩ	1.7 μΩ/Ω	0.9999948 kΩ	1.0000150 kΩ	
20 kOhm Range (4W)						
10.000000 kOhm	10.0000538 kΩ	10.000049 kΩ	1.4 μΩ/Ω	9.999953 kΩ	10.000155 kΩ	
200 kOhm Range (4W)						
100.00000 kOhm	99.999557 kΩ	99.99945 kΩ	2.5 μΩ/Ω	99.99855 kΩ	100.00057 kΩ	
2 MOhm Range (4W)						
1.0000000 MOhm	0.99997977 MΩ	0.9999789 MΩ	4.3 μΩ/Ω	0.9999681 MΩ	0.9999915 MΩ	
20 MOhm Range (4W)						
10.000000 MOhm	9.9990359 MΩ	9.998995 MΩ	12.0 μΩ/Ω	9.998716 MΩ	9.999356 MΩ	
200 MOhm Range (2W)						
100.0000 MOhm	100.042286 MΩ	100.04156 MΩ	45.0 μΩ/Ω	100.02278 MΩ	100.06179 MΩ	
2 GOhm Range (2W)						
1.000000 GOhm	1.00009390 GΩ	0.9994291 GΩ	350.0 μΩ/Ω	0.9982188 GΩ	1.0019690 GΩ	
Normal Ohms Lol Verification						
2 Ohm Range (4W)						
1.0000000 Ohm	0.99975691 Ω	0.9997601 Ω	8.1 μΩ/Ω	0.9997329 Ω	0.9997809 Ω	
20 Ohm Range (4W)						
10.000000 Ohm	9.9999336 Ω	9.999920 Ω	3.0 μΩ/Ω	9.999801 Ω	10.000067 Ω	
200 Ohm Range (4W)						
100.00000 Ohm	100.002138 Ω	100.00186 Ω	2.5 μΩ/Ω	100.00101 Ω	100.00327 Ω	
2 kOhm Range (4W)						
1.0000000 kOhm	1.00000494 kΩ	1.0000007 kΩ	2.5 μΩ/Ω	0.9999936 kΩ	1.0000162 kΩ	
20 kOhm Range (4W)						
10.000000 kOhm	10.0000538 kΩ	10.000013 kΩ	2.5 μΩ/Ω	9.999941 kΩ	10.000167 kΩ	
200 kOhm Range (4W)						
100.00000 kOhm	99.999557 kΩ	99.99956 kΩ	1.6 μΩ/Ω	99.99849 kΩ	100.00063 kΩ	
2 MOhm Range (4W)						
1.0000000 MOhm	0.99997977 MΩ	0.9999778 MΩ	4.5 μΩ/Ω	0.9999656 MΩ	0.9999940 MΩ	

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
				Lower Limit	Upper Limit	
20 MOhm Range (4W)						
10.000000 MOhm	9.9990359 MΩ	9.998853 MΩ	14.0 μΩ/Ω	9.998466 MΩ	9.999606 MΩ	
200 MOhm Range (2W)						
100.0000 MOhm	100.042286 MΩ	100.03319 MΩ	300.0 μΩ/Ω	99.85526 MΩ	100.22931 MΩ	
2 GOhm Range (2W)						
1.000000 GOhm	1.00009390 GΩ	0.9996362 GΩ	400.0 μΩ/Ω	0.9982188 GΩ	1.0019690 GΩ	
True Ohms Verification						
2 Ohm Range (4W)						
1.0000000 Ohm	0.99975691 Ω	0.9997623 Ω	8.6 μΩ/Ω	0.9997329 Ω	0.9997809 Ω	
20 Ohm Range (4W)						
10.000000 Ohm	9.9999336 Ω	9.999928 Ω	2.5 μΩ/Ω	9.999801 Ω	10.000067 Ω	
200 Ohm Range (4W)						
100.00000 Ohm	100.002138 Ω	100.00211 Ω	2.5 μΩ/Ω	100.00113 Ω	100.00315 Ω	
2 kOhm Range (4W)						
1.0000000 kOhm	1.00000494 kΩ	1.0000046 kΩ	1.5 μΩ/Ω	0.9999948 kΩ	1.0000150 kΩ	
20 kOhm Range (4W)						
10.000000 kOhm	10.0000538 kΩ	10.000047 kΩ	1.5 μΩ/Ω	9.999953 kΩ	10.000155 kΩ	
True Ohms LoI Verification						
2 Ohm Range (4W)						
1.0000000 Ohm	0.99975691 Ω	0.9997623 Ω	9.1 μΩ/Ω	0.9997329 Ω	0.9997809 Ω	
20 Ohm Range (4W)						
10.000000 Ohm	9.9999336 Ω	9.999929 Ω	2.5 μΩ/Ω	9.999801 Ω	10.000067 Ω	
200 Ohm Range (4W)						
100.00000 Ohm	100.002138 Ω	100.00209 Ω	2.5 μΩ/Ω	100.00101 Ω	100.00327 Ω	
2 kOhm Range (4W)						
1.0000000 kOhm	1.00000494 kΩ	1.0000037 kΩ	1.5 μΩ/Ω	0.9999936 kΩ	1.0000162 kΩ	
20 kOhm Range (4W)						
10.000000 kOhm	10.0000538 kΩ	10.000042 kΩ	2.0 μΩ/Ω	9.999941 kΩ	10.000167 kΩ	
HI Voltage Ohms Verification						
20 MOhm Range (4W)						
10.000000 MOhm	9.9990359 MΩ	9.999002 MΩ	12.0 μΩ/Ω	9.998834 MΩ	9.999238 MΩ	
200 MOhm Range (2W)						
100.0000 MOhm	100.042286 MΩ	100.04538 MΩ	21.0 μΩ/Ω	100.03358 MΩ	100.05099 MΩ	
2 GOhm Range (2W)						
1.000000 GOhm	1.0000939 GΩ	1.000254 GΩ	50.0 μΩ/Ω	0.999779 GΩ	1.000409 GΩ	
20 GOhm Range (2W)						
10.000000 GOhm	10.000891 GΩ	10.01038 GΩ	280.0 μΩ/Ω	9.98214 GΩ	10.01964 GΩ	
DC Voltage Verification						

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
200 mV Range						
100.00000 mV	99.999991 mV	99.99998 mV	3.2 μV/V	99.99927 mV	100.00071 mV	
-100.00000 mV	-100.000089 mV	-100.00019 mV	3.2 μV/V	-100.00081 mV	-99.99937 mV	
2 V Range						
1.0000000 V	1.00000025 V	0.9999998 V	1.0 μV/V	0.9999958 V	1.0000048 V	
-1.0000000 V	-1.00000028 V	-1.0000001 V	1.0 μV/V	-1.0000048 V	-0.9999958 V	
20 V Range						
0.000010 V	0.0000099 V	0.000011 V	110000.0 μV/V	0.000005 V	0.000015 V	
-0.000010 V	-0.0000101 V	-0.000009 V	120000.0 μV/V	-0.000015 V	-0.000005 V	
0.000100 V	0.0000999 V	0.000101 V	15000.0 μV/V	0.000095 V	0.000105 V	
-0.000100 V	-0.0001001 V	-0.000099 V	15000.0 μV/V	-0.000105 V	-0.000095 V	
0.001000 V	0.0009999 V	0.001001 V	1300.0 μV/V	0.000995 V	0.001005 V	
-0.001000 V	-0.0010001 V	-0.000999 V	1500.0 μV/V	-0.001005 V	-0.000995 V	
0.010000 V	0.0099999 V	0.010001 V	130.0 μV/V	0.009995 V	0.010005 V	
-0.010000 V	-0.0100001 V	-0.009999 V	150.0 μV/V	-0.010005 V	-0.009995 V	
0.100000 V	0.1000000 V	0.100001 V	10.0 μV/V	0.099995 V	0.100005 V	
-0.100000 V	-0.1000001 V	-0.099999 V	13.0 μV/V	-0.100005 V	-0.099995 V	
1.000000 V	1.0000003 V	1.000001 V	1.5 μV/V	0.999991 V	1.000009 V	
-1.000000 V	-1.0000003 V	-0.999999 V	1.5 μV/V	-1.000009 V	-0.999991 V	
5.000000 V	4.9999987 V	5.000001 V	0.9 μV/V	4.999974 V	5.000024 V	
-5.000000 V	-4.9999997 V	-4.999999 V	0.9 μV/V	-5.000025 V	-4.999975 V	
10.000000 V	9.9999974 V	10.000000 V	0.6 μV/V	9.999952 V	10.000042 V	
-10.000000 V	-9.9999994 V	-10.000000 V	0.6 μV/V	-10.000044 V	-9.999954 V	
15.000000 V	14.9999978 V	14.999999 V	0.9 μV/V	14.999933 V	15.000063 V	
-15.000000 V	-14.9999983 V	-14.999999 V	0.6 μV/V	-15.000063 V	-14.999933 V	
19.000000 V	18.9999972 V	18.999999 V	0.7 μV/V	18.999916 V	19.000078 V	
-19.000000 V	-18.9999979 V	-18.999998 V	0.7 μV/V	-19.000079 V	-18.999917 V	
200 V Range						
100.00000 V	100.000021 V	100.00005 V	0.8 μV/V	99.99937 V	100.00067 V	
-100.00000 V	-100.000023 V	-100.00003 V	0.8 μV/V	-100.00067 V	-99.99937 V	
1000 V Range						
1000.0000 V	999.99833 V	1000.0006 V	0.9 μV/V	999.9917 V	1000.0049 V	
-1000.0000 V	-999.99810 V	-1000.0001 V	0.9 μV/V	-1000.0047 V	-999.9915 V	
AC Voltage Verification						
200 mV Range						
100.0000 mV @ 20 Hz	99.99858 mV	100.0021 mV	75.0 μV/V	99.9791 mV	100.0181 mV	
100.0000 mV @ 55 Hz	99.99827 mV	100.0015 mV	38.0 μV/V	99.9808 mV	100.0158 mV	
100.0000 mV @ 300 Hz	99.99915 mV	100.0003 mV	45.0 μV/V	99.9842 mV	100.0140 mV	

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
				Lower Limit	Upper Limit	
10.0000 mV @ 1 kHz	9.99852 mV	9.9991 mV	240.0 μV/V	9.9949 mV	10.0022 mV	
100.0000 mV @ 1 kHz	99.99887 mV	99.9999 mV	36.0 μV/V	99.9840 mV	100.0138 mV	
100.0000 mV @ 3 kHz	99.99982 mV	99.9990 mV	42.0 μV/V	99.9823 mV	100.0173 mV	
100.0000 mV @ 10 kHz	100.00017 mV	100.0012 mV	35.0 μV/V	99.9827 mV	100.0177 mV	
100.0000 mV @ 30 kHz	100.00005 mV	99.9943 mV	72.0 μV/V	99.9555 mV	100.0445 mV	
100.0000 mV @ 60 kHz	100.00182 mV	99.9958 mV	120.0 μV/V	99.9023 mV	100.1013 mV	
100.0000 mV @ 100 kHz	100.00349 mV	99.9974 mV	120.0 μV/V	99.9040 mV	100.1030 mV	
2 V Range						
1.000000 V @ 20 Hz	1.0000086 V	1.000026 V	43.0 μV/V	0.999865 V	1.000153 V	
1.000000 V @ 55 Hz	0.9999971 V	1.000020 V	44.0 μV/V	0.999878 V	1.000116 V	
1.000000 V @ 300 Hz	1.0000032 V	1.000007 V	20.0 μV/V	0.999904 V	1.000102 V	
0.010000 V @ 1 kHz	0.0099985 V	0.009998 V	300.0 μV/V	0.009974 V	0.010023 V	
1.000000 V @ 1 kHz	1.0000037 V	1.000005 V	23.0 μV/V	0.999905 V	1.000103 V	
1.000000 V @ 3 kHz	1.0000041 V	0.999994 V	23.0 μV/V	0.999885 V	1.000123 V	
1.000000 V @ 10 kHz	1.0000059 V	1.000004 V	26.0 μV/V	0.999887 V	1.000125 V	
1.000000 V @ 30 kHz	1.0000041 V	0.999985 V	58.0 μV/V	0.999709 V	1.000299 V	
1.000000 V @ 60 kHz	0.9999933 V	1.000009 V	84.0 μV/V	0.999198 V	1.000788 V	
1.000000 V @ 100 kHz	0.9999844 V	1.000019 V	130.0 μV/V	0.999189 V	1.000779 V	
1.000000 V @ 500 kHz	0.9999194 V	0.999592 V	600.0 μV/V	0.965920 V	1.033919 V	
1.000000 V @ 1 MHz	0.9997295 V	1.001748 V	2500.0 μV/V	0.965732 V	1.033727 V	
20 V Range						
10.00000 V @ 20 Hz	10.000150 V	10.00020 V	45.0 μV/V	9.99871 V	10.00159 V	
10.00000 V @ 55 Hz	10.000012 V	10.00015 V	29.0 μV/V	9.99882 V	10.00120 V	
10.00000 V @ 300 Hz	10.000034 V	10.00012 V	25.0 μV/V	9.99904 V	10.00102 V	
0.10000 V @ 1 kHz	0.099999 V	0.09999 V	400.0 μV/V	0.09975 V	0.10025 V	
1.00000 V @ 1 kHz	1.000004 V	1.00008 V	40.0 μV/V	0.99969 V	1.00032 V	
10.00000 V @ 1 kHz	10.000023 V	10.00004 V	25.0 μV/V	9.99903 V	10.00101 V	
10.00000 V @ 1 kHz	19.000007 V	18.99995 V	18.0 μV/V	18.99834 V	19.00167 V	
10.00000 V @ 3 kHz	10.000019 V	9.99984 V	25.0 μV/V	9.99883 V	10.00121 V	
10.00000 V @ 10 kHz	10.000032 V	10.00006 V	25.0 μV/V	9.99884 V	10.00122 V	
10.00000 V @ 30 kHz	10.000089 V	10.00024 V	25.0 μV/V	9.99714 V	10.00304 V	
10.00000 V @ 60 kHz	10.000156 V	10.00053 V	50.0 μV/V	9.99221 V	10.00811 V	
10.00000 V @ 100 kHz	9.999827 V	10.00046 V	80.0 μV/V	9.99188 V	10.00778 V	
10.00000 V @ 500 kHz	9.999939 V	10.03612 V	400.0 μV/V	9.65994 V	10.33994 V	
10.00000 V @ 1 MHz	10.000578 V	9.92075 V	2500.0 μV/V	9.66057 V	10.34058 V	
200 V Range						
100.0000 V @ 20 Hz	99.99941 V	99.9997 V	50.0 μV/V	99.9850 V	100.0138 V	
100.0000 V @ 55 Hz	99.99816 V	99.9988 V	39.0 μV/V	99.9863 V	100.0101 V	

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
				Lower Limit	Upper Limit	
100.0000 V @ 300 Hz	99.99880 V	99.9986 V	31.0 μ V/V	99.9889 V	100.0087 V	
1.0000 V @ 1 kHz	1.00000 V	0.9999 V	400.0 μ V/V	0.9975 V	1.0025 V	
100.0000 V @ 1 kHz	99.99850 V	99.9980 V	35.0 μ V/V	99.9886 V	100.0084 V	
100.0000 V @ 3 kHz	99.99850 V	99.9957 V	37.0 μ V/V	99.9867 V	100.0105 V	
100.0000 V @ 10 kHz	99.99893 V	99.9964 V	37.0 μ V/V	99.9870 V	100.0108 V	
100.0000 V @ 30 kHz	100.00101 V	100.0005 V	30.0 μ V/V	99.9715 V	100.0305 V	
100.0000 V @ 60 kHz	100.00482 V	100.0085 V	40.0 μ V/V	99.9253 V	100.0843 V	
100.0000 V @ 100 kHz	100.00252 V	100.0167 V	120.0 μ V/V	99.9230 V	100.0820 V	

1000 V Range

500.000 V @ 55 Hz	500.0043 V	500.008 V	35.0 μ V/V	499.916 V	500.092 V	
500.000 V @ 300 Hz	500.0128 V	500.012 V	31.0 μ V/V	499.925 V	500.101 V	
5.000 V @ 1 kHz	5.0000 V	5.000 V	400.0 μ V/V	4.974 V	5.026 V	
500.000 V @ 1 kHz	500.0098 V	500.012 V	25.0 μ V/V	499.922 V	500.098 V	
500.000 V @ 3 kHz	500.0061 V	499.996 V	25.0 μ V/V	499.918 V	500.094 V	
500.000 V @ 10 kHz	500.0055 V	500.007 V	26.0 μ V/V	499.917 V	500.093 V	
500.000 V @ 30 kHz	500.0331 V	500.046 V	90.0 μ V/V	499.810 V	500.256 V	
1000.0000 V @ 55 Hz	1000.00485 V	999.9695 V	31.0 μ V/V	999.6738 V	1000.3358 V	
1000.000 V @ 300 Hz	1000.0225 V	1000.017 V	80.0 μ V/V	999.691 V	1000.353 V	
1000.000 V @ 1 kHz	1000.0203 V	1000.013 V	74.0 μ V/V	999.689 V	1000.351 V	
1000.000 V @ 3 kHz	1000.0048 V	999.979 V	75.0 μ V/V	999.674 V	1000.336 V	
1000.000 V @ 10 kHz	1000.0047 V	1000.015 V	110.0 μ V/V	999.674 V	1000.336 V	
1000.000 V @ 30 kHz	1000.0913 V	1000.237 V	310.0 μ V/V	998.615 V	1001.567 V	

DC Current Verification

200 μ A Range

100.00000 μ A	99.998882 μ A	99.99949 μ A	5.0 μ A/A	99.99698 μ A	100.00078 μ A	
-100.00000 μ A	-99.999668 μ A	-99.99976 μ A	5.0 μ A/A	-100.00157 μ A	-99.99777 μ A	

2 mA Range

1.0000000 mA	0.99999870 mA	0.9999979 mA	4.7 μ A/A	0.9999797 mA	1.0000177 mA	
-1.0000000 mA	-0.99999846 mA	-1.0000040 mA	4.7 μ A/A	-1.0000175 mA	-0.9999795 mA	

20 mA Range

10.0000000 mA	9.9999610 mA	9.999979 mA	3.8 μ A/A	9.999761 mA	10.000161 mA	
-10.0000000 mA	-9.9999625 mA	-10.000001 mA	3.8 μ A/A	-10.000162 mA	-9.999762 mA	

200 mA Range

100.00000 mA	100.000306 mA	100.00073 mA	11.0 μ A/A	99.99501 mA	100.00561 mA	
-100.00000 mA	-100.000094 mA	-100.00001 mA	11.0 μ A/A	-100.00539 mA	-99.99479 mA	

2 A Range

1.0000000 A	1.00000212 A	1.0000077 A	14.0 μ A/A	0.9997761 A	1.0002281 A	
-1.0000000 A	-0.99999948 A	-1.0000043 A	14.0 μ A/A	-1.0002255 A	-0.9997735 A	

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
				Lower Limit	Upper Limit	
20 A Range						
10.000000 A	10.0004068 A	10.000600 A	100.0 μA/A	9.995457 A	10.005357 A	
-10.000000 A	-10.0002870 A	-10.000226 A	100.0 μA/A	-10.005237 A	-9.995337 A	
AC Current Verification						
200 uA Range						
100.0000 μA @ 55 Hz	99.99933 μA	99.9958 μA	100.0 μA/A	99.9163 μA	100.0823 μA	
10.0000 μA @ 300 Hz	10.00042 μA	10.0004 μA	790.0 μA/A	9.9705 μA	10.0303 μA	
100.0000 μA @ 300 Hz	99.99947 μA	99.9988 μA	60.0 μA/A	99.9165 μA	100.0825 μA	
100.0000 μA @ 1 kHz	99.99900 μA	99.9968 μA	60.0 μA/A	99.9160 μA	100.0820 μA	
100.0000 μA @ 5 kHz	99.98432 μA	99.9890 μA	190.0 μA/A	99.9013 μA	100.0673 μA	
100.0000 μA @ 10 kHz	99.93920 μA	99.9779 μA	200.0 μA/A	99.8562 μA	100.0222 μA	
2 mA Range						
1.000000 mA @ 55 Hz	1.0000017 mA	0.999959 mA	100.0 μA/A	0.999422 mA	1.000582 mA	
0.010000 mA @ 300 Hz	0.0100004 mA	0.009998 mA	1500.0 μA/A	0.009757 mA	0.010244 mA	
1.000000 mA @ 300 Hz	1.0000010 mA	0.999992 mA	40.0 μA/A	0.999421 mA	1.000581 mA	
1.000000 mA @ 1 kHz	0.9999956 mA	0.999973 mA	45.0 μA/A	0.999416 mA	1.000576 mA	
1.000000 mA @ 5 kHz	1.0000147 mA	0.999931 mA	65.0 μA/A	0.999435 mA	1.000595 mA	
1.000000 mA @ 10 kHz	0.9999590 mA	0.999836 mA	95.0 μA/A	0.999379 mA	1.000539 mA	
20 mA Range						
10.00000 mA @ 55 Hz	9.999647 mA	9.99932 mA	100.0 μA/A	9.99385 mA	10.00545 mA	
0.10000 mA @ 300 Hz	0.0999999 mA	0.09998 mA	1400.0 μA/A	0.09757 mA	0.10243 mA	
10.00000 mA @ 300 Hz	9.999657 mA	9.99964 mA	40.0 μA/A	9.99386 mA	10.00546 mA	
10.00000 mA @ 1 kHz	9.999575 mA	9.99949 mA	40.0 μA/A	9.99377 mA	10.00537 mA	
10.00000 mA @ 5 kHz	10.000258 mA	9.99977 mA	100.0 μA/A	9.99446 mA	10.00606 mA	
10.00000 mA @ 10 kHz	10.001466 mA	10.00010 mA	120.0 μA/A	9.99567 mA	10.00727 mA	
200 mA Range						
100.0000 mA @ 55 Hz	99.99672 mA	99.9930 mA	100.0 μA/A	99.9422 mA	100.0512 mA	
10.0000 mA @ 300 Hz	9.99966 mA	9.9992 mA	110.0 μA/A	9.9726 mA	10.0267 mA	
100.0000 mA @ 300 Hz	99.99669 mA	99.9965 mA	40.0 μA/A	99.9422 mA	100.0512 mA	
100.0000 mA @ 1 kHz	99.99601 mA	99.9944 mA	40.0 μA/A	99.9415 mA	100.0505 mA	
100.0000 mA @ 5 kHz	100.00109 mA	99.9993 mA	100.0 μA/A	99.9466 mA	100.0556 mA	
100.0000 mA @ 10 kHz	100.01742 mA	100.0086 mA	110.0 μA/A	99.9629 mA	100.0719 mA	
2 A Range						
1.000000 A @ 55 Hz	0.9999732 A	0.999942 A	100.0 μA/A	0.999028 A	1.000918 A	
0.100000 A @ 300 Hz	0.0999967 A	0.099996 A	140.0 μA/A	0.099686 A	0.100307 A	
1.000000 A @ 300 Hz	0.9999714 A	0.999980 A	50.0 μA/A	0.999026 A	1.000916 A	
1.000000 A @ 1 kHz	0.9999870 A	1.000036 A	40.0 μA/A	0.999042 A	1.000932 A	
1.000000 A @ 5 kHz	1.0001522 A	1.000461 A	210.0 μA/A	0.999097 A	1.001207 A	

Certificate Number: EVL1035363

Date of Calibration: 01 Mar 2025

Calibration Results

Nominal Value	Reference Value	Measurement Result	Expanded Uncertainty	Limits of Error		Status
				Lower Limit	Upper Limit	
1.000000 A @ 10 kHz	1.0008686 A	1.001226 A	520.0 μA/A	0.999813 A	1.001924 A	
20 A Range						
1.00000 A @ 300 Hz	0.999971 A	0.99995 A	140.0 μA/A	0.99667 A	1.00327 A	
10.00000 A @ 55 Hz	10.000472 A	10.00039 A	160.0 μA/A	9.98907 A	10.01187 A	
10.00000 A @ 300 Hz	10.000740 A	10.00081 A	120.0 μA/A	9.98934 A	10.01214 A	
10.00000 A @ 1 kHz	10.001538 A	10.00149 A	90.0 μA/A	9.99014 A	10.01294 A	
10.00000 A @ 5 kHz	10.003084 A	10.00956 A	550.0 μA/A	9.97568 A	10.03049 A	
10.00000 A @ 10 kHz	10.004649 A	10.01143 A	700.0 μA/A	9.97724 A	10.03206 A	
Frequency Verification						
1.000000 MHz	1.000000 MHz	1.0000000 MHz	1.3 μHz/Hz	0.9999880 MHz	1.0000120 MHz	