



Calibration Cert# 2166.01

FLUKE

Certificate of Calibration

Everett Service Center

Certificate Number: EVL769023

Data Type: As-Left
Result Summary: Measurement Results < Limits
Manufacturer: Fluke
Model: 8508A
Serial Number: 276568089
Description: Reference Multimeter
Option(s): 01

Calibration Date: 24-Jan-2022
Calibration Due: 24-Jan-2024
Certificate Date: 25-Jan-2022
Temperature: 22.2 °C
Humidity: 37.1 %

Procedure: Fluke 8508A ACAL/ZCAL VER 5720A/5725A

Revision: 20190531

Customer: MODERN SURVEYING CALIBRATION & TESTING LABS(FZE)
City: ERBIL

Country: IQ

Purchase Order: PO1217064

RMA: 32324785

This calibration is traceable to the International System of Units (SI), through National Metrology Institutes (NIST, PTB, NRC, NPL, etc.), radiometric techniques, or natural physical constants. This certificate applies only to the item identified and shall not be reproduced other than in full, without the specific written approval by Fluke Corporation. Calibration certificates without signature are not valid. The calibration has been completed in accordance with Fluke Electronics Corporation Quality System Document 111.0 Revision 124 and/or Fluke 17025 Quality Manual QSD 111.41 Revision 007.

The Data Type found in this certificate must be interpreted as:

- As - Found Calibration data collected before the unit is adjusted and / or repaired.
- As - Left Calibration data collected after the unit has been adjusted and / or repaired.
- Found-Left Calibration data collected without any adjustment and / or repair performed.

This calibration conforms to the requirements of ISO/IEC 17025:2017 and ANSI/NCCL Z540-1-1994 (R2002).

In the attached measurement results, deviation may be expressed with units, Measured Value (MV) - Nominal Value (NV) or as a proportion of the nominal value ((MV-NV)/NV), expressed without units with a scalar multiplier such as % (0.01), or as a ratio of the units (mA/A, μ V/V, etc.) Descriptions such as μ A/A, μ V/V, and others, where used to annotate results or column headings are the preferred replacements for what was historically labeled as "ppm" or parts-per-million and described the results in that column, unless otherwise noted by units symbols.


Where applicable, the expanded uncertainty of measurement at the time of test is given in the following pages. They are calculated in accordance with the method described in the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k , such that the confidence level approximates 95%.


This calibration certificate may contain data that is not covered by the A2LA Scope of Accreditation. Unaccredited material, where applicable is indicated by an asterisk (*), or confined to clearly marked sections. Functional (Pass / Fail) tests are not accredited.

No statement of compliance with specifications is made or implied on this certificate. However, measurement results are reviewed, where applicable, to establish where any measurement result exceeded the manufacturer's specifications.

Measurement results greater than limits of error are indicated by '!'.

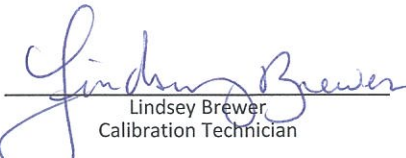


Lindsey Brewer
Calibration Technician

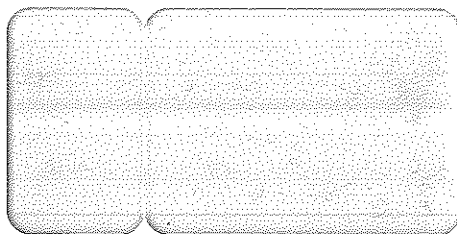

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Standards Used

Asset	Description	Cal-Date	Cal-Due
L101S	Fluke 5720A / 5725A Characterized Set	18-Jan-2022	18-Feb-2022
J680	Fluke 5725A Amplifier	18-Jan-2022	18-Jan-2023
1610S	Fluke 910R GPS Frequency Standard	12-Feb-2021	12-Feb-2022
J1169	Measurements International 9331G/100M Standard Resistor	10-Jun-2021	10-Jun-2022
J1675	Measurements International 9331G/1G Standard Resistor	29-Jun-2021	29-Jun-2022
15659	Ohm-Labs 110 10 GOhm High Resistance Standard	26-Apr-2021	26-Apr-2022
J1346	Stanford Research Systems DS345 Synthesized Function Generator	18-Jan-2022	18-Jan-2023

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
8508A 1 Year Verification (99% Specification)					
UUT Firmware Version : 03.05					
Normal Ohms Verification					
2 Ohm Range (4W)					
1.0000000 Ohm	0.99989499	0.9998909	0.9998710	0.9999190	8.1 μΩ/Ω
20 Ohm Range (4W)					
10.0000000 Ohm	10.0003051	10.000294	10.000172	10.000438	2.5 μΩ/Ω
200 Ohm Range (4W)					
100.000000 Ohm	100.003734	100.00369	100.00272	100.00474	2.4 μΩ/Ω
2 kOhm Range (4W)					
1.0000000 kOhm	1.00000737	1.0000071	0.9999973	1.0000175	1.7 μΩ/Ω
20 kOhm Range (4W)					
10.0000000 kOhm	9.9999140	9.999905	9.999813	10.000015	1.4 μΩ/Ω
200 kOhm Range (4W)					
100.000000 kOhm	99.998644	99.99854	99.99763	99.99965	2.5 μΩ/Ω
2 MOhm Range (4W)					
1.0000000 MOhm	0.99997185	0.9999672	0.9999602	0.9999836	4.3 μΩ/Ω
20 MOhm Range (4W)					
10.0000000 MOhm	9.9991709	9.999171	9.998851	9.999491	11.5 μΩ/Ω
200 MOhm Range (2W)					
100.00000 MOhm	100.004282	100.00451	99.98478	100.02378	45.0 μΩ/Ω
2 GOhm Range (2W)					
1.0000000 GOhm	1.00007214	1.0002247	0.9981971	1.0019472	350.0 μΩ/Ω
Normal Ohms Lol Verification					
2 Ohm Range (4W)					
1.0000000 Ohm	0.99989499	0.9998954	0.9998710	0.9999190	8.1 μΩ/Ω
20 Ohm Range (4W)					
10.0000000 Ohm	10.0003051	10.000308	10.000172	10.000438	3.0 μΩ/Ω
200 Ohm Range (4W)					
100.000000 Ohm	100.003734	100.00378	100.00260	100.00486	2.5 μΩ/Ω
2 kOhm Range (4W)					
1.0000000 kOhm	1.00000737	1.0000078	0.9999961	1.0000187	2.5 μΩ/Ω
20 kOhm Range (4W)					
10.0000000 kOhm	9.9999140	9.999905	9.999801	10.000027	2.5 μΩ/Ω
200 kOhm Range (4W)					

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
100.00000 kOhm	99.998644	99.99863	99.99757	99.99971	1.6 μΩ/Ω
2 MOhm Range (4W)					
1.0000000 MOhm	0.99997185	0.9999718	0.9999577	0.9999861	4.5 μΩ/Ω
20 MOhm Range (4W)					
10.000000 MOhm	9.9991709	9.999181	9.998601	9.999741	14.0 μΩ/Ω
200 MOhm Range (2W)					
100.0000 MOhm	100.004282	100.00390	99.81728	100.19128	300.0 μΩ/Ω
2 GOhm Range (2W)					
1.000000 GOhm	1.00007214	1.0001810	0.9981971	1.0019472	400.0 μΩ/Ω
True Ohms Verification					
2 Ohm Range (4W)					
1.0000000 Ohm	0.99989499	0.9998905	0.9998710	0.9999190	8.6 μΩ/Ω
20 Ohm Range (4W)					
10.000000 Ohm	10.0003051	10.000284	10.000172	10.000438	2.5 μΩ/Ω
200 Ohm Range (4W)					
100.00000 Ohm	100.003734	100.00363	100.00272	100.00474	2.5 μΩ/Ω
2 kOhm Range (4W)					
1.0000000 kOhm	1.00000737	1.0000069	0.9999973	1.0000175	1.5 μΩ/Ω
20 kOhm Range (4W)					
10.000000 kOhm	9.9999140	9.999904	9.999813	10.000015	1.5 μΩ/Ω
True Ohms Lol Verification					
2 Ohm Range (4W)					
1.0000000 Ohm	0.99989499	0.9998911	0.9998710	0.9999190	9.1 μΩ/Ω
20 Ohm Range (4W)					
10.000000 Ohm	10.0003051	10.000294	10.000172	10.000438	2.5 μΩ/Ω
200 Ohm Range (4W)					
100.00000 Ohm	100.003734	100.00349	100.00260	100.00486	2.5 μΩ/Ω
2 kOhm Range (4W)					
1.0000000 kOhm	1.00000737	1.0000066	0.9999961	1.0000187	1.5 μΩ/Ω
20 kOhm Range (4W)					
10.000000 kOhm	9.9999140	9.999903	9.999801	10.000027	2.0 μΩ/Ω
HI Voltage Ohms Verification					
20 MOhm Range (4W)					
10.000000 MOhm	9.9991709	9.999158	9.998969	9.999373	11.5 μΩ/Ω
200 MOhm Range (2W)					

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
100.0000 MOhm	100.004282	100.00475	99.99558	100.01298	21.0 μΩ/Ω
2 GOhm Range (2W)					
1.000000 GOhm	1.0000721	1.000094	0.999757	1.000387	50.0 μΩ/Ω
20 GOhm Range (2W)					
10.000000 GOhm	10.000844	10.00258	9.98209	10.01959	280.0 μΩ/Ω
DC Voltage Verification					
200 mV Range					
100.00000 mV	99.999182	99.99916	99.99846	99.99990	3.2 μV/V
-100.00000 mV	-99.999347	-99.99942	-100.00007	-99.99863	3.2 μV/V
2 V Range					
1.0000000 V	0.99999745	0.9999970	0.9999929	1.0000019	1.0 μV/V
-1.0000000 V	-0.99999760	-0.9999973	-1.0000021	-0.9999931	1.0 μV/V
20 V Range					
0.000010 V	0.0000099	0.000011	0.000005	0.000015	106,000.0 μV/V
-0.000010 V	-0.0000101	-0.000009	-0.000015	-0.000005	120,000.0 μV/V
0.000100 V	0.0000999	0.000102	0.000095	0.000105	15,400.0 μV/V
-0.000100 V	-0.0001001	-0.000098	-0.000105	-0.000095	15,400.0 μV/V
0.001000 V	0.0009999	0.001002	0.000995	0.001005	1,270.0 μV/V
-0.001000 V	-0.0010001	-0.000998	-0.001005	-0.000995	1,540.0 μV/V
0.010000 V	0.0099998	0.010002	0.009995	0.010005	129.0 μV/V
-0.010000 V	-0.0100000	-0.009998	-0.010005	-0.009995	152.0 μV/V
0.100000 V	0.0999992	0.100001	0.099994	0.100005	10.0 μV/V
-0.100000 V	-0.0999993	-0.099998	-0.100005	-0.099994	12.7 μV/V
1.000000 V	0.9999974	0.999999	0.999988	1.000006	1.5 μV/V
-1.000000 V	-0.9999976	-0.999997	-1.000007	-0.999989	1.5 μV/V
5.000000 V	4.9999904	4.999989	4.999965	5.000015	0.90 μV/V
-5.000000 V	-4.9999911	-4.999989	-5.000016	-4.999966	0.90 μV/V
10.000000 V	9.9999807	9.999977	9.999936	10.000026	0.60 μV/V
-10.000000 V	-9.9999823	-9.999979	-10.000027	-9.999937	0.60 μV/V
15.000000 V	14.9999759	14.999972	14.999911	15.000041	0.90 μV/V
-15.000000 V	-14.9999804	-14.999975	-15.000045	-14.999915	0.60 μV/V
19.000000 V	18.9999694	18.999963	18.999888	19.000050	0.70 μV/V
-19.000000 V	-18.9999752	-18.999969	-19.000056	-18.999894	0.70 μV/V
200 V Range					
100.00000 V	99.999928	99.99991	99.99928	100.00058	0.80 μV/V
Fluke Corporation	Telephone	Facsimile	Internet		Revision 2.19
1420 75th St SW, Everett WA 98203 USA	888.993.5853	425.446.6390	www.fluke.com		

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
-100.00000 V	-99.999917	-99.99987	-100.00057	-99.99927	0.80 μ V/V
1000 V Range					
1000.0000 V	1000.00149	1000.0013	999.9949	1000.0081	0.90 μ V/V
-1000.0000 V	-1000.00127	-1000.0008	-1000.0079	-999.9947	0.90 μ V/V
AC Voltage Verification					
200 mV Range					
100.0000 mV @ 20 Hz	99.99927	100.0011	99.9798	100.0188	75.0 μ V/V
100.0000 mV @ 55 Hz	99.99877	100.0003	99.9813	100.0163	38.0 μ V/V
100.0000 mV @ 300 Hz	99.99860	99.9987	99.9837	100.0135	45.0 μ V/V
10.0000 mV @ 1 kHz	9.99865	9.9984	9.9950	10.0023	238.0 μ V/V
100.0000 mV @ 1 kHz	99.99858	99.9985	99.9837	100.0135	36.0 μ V/V
100.0000 mV @ 3 kHz	99.99893	99.9976	99.9814	100.0164	42.0 μ V/V
100.0000 mV @ 10 kHz	99.99952	100.0003	99.9820	100.0170	35.0 μ V/V
100.0000 mV @ 30 kHz	100.00036	99.9937	99.9559	100.0449	72.0 μ V/V
100.0000 mV @ 60 kHz	100.00152	99.9957	99.9020	100.1010	116.0 μ V/V
100.0000 mV @ 100 kHz	100.00504	99.9992	99.9055	100.1045	118.0 μ V/V
2 V Range					
1.000000 V @ 20 Hz	1.0000037	1.000022	0.999860	1.000148	43.0 μ V/V
1.000000 V @ 55 Hz	1.0000002	1.000016	0.999881	1.000119	44.0 μ V/V
1.000000 V @ 300 Hz	0.9999990	1.000001	0.999900	1.000098	20.0 μ V/V
0.010000 V @ 1 kHz	0.0099986	0.009999	0.009974	0.010023	300.0 μ V/V
1.000000 V @ 1 kHz	0.9999994	0.999998	0.999900	1.000098	23.0 μ V/V
1.000000 V @ 3 kHz	1.0000019	0.999987	0.999883	1.000121	23.0 μ V/V
1.000000 V @ 10 kHz	1.0000022	0.999998	0.999883	1.000121	26.0 μ V/V
1.000000 V @ 30 kHz	0.9999999	0.999983	0.999705	1.000295	58.0 μ V/V
1.000000 V @ 60 kHz	0.9999930	1.000006	0.999198	1.000788	84.0 μ V/V
1.000000 V @ 100 kHz	0.9999748	1.000013	0.999180	1.000770	132.0 μ V/V
1.000000 V @ 500 kHz	0.9997577	0.999464	0.965760	1.033755	600.0 μ V/V
1.000000 V @ 1 MHz	0.9990530	1.001056	0.965062	1.033044	2,500.0 μ V/V
20 V Range					
10.00000 V @ 20 Hz	10.000106	10.00016	9.99867	10.00155	45.0 μ V/V
10.00000 V @ 55 Hz	10.000018	10.00010	9.99883	10.00121	29.0 μ V/V
10.00000 V @ 300 Hz	10.000002	10.00005	9.99901	10.00099	25.0 μ V/V
0.10000 V @ 1 kHz	0.099999	0.10000	0.09975	0.10025	400.0 μ V/V
1.00000 V @ 1 kHz	0.999999	1.00007	0.99968	1.00031	40.0 μ V/V

Fluke Corporation
Telephone
Facsimile
Internet
Revision
2.19

1420 75th St SW, Everett WA 98203 USA

888.993.5853

425.446.6390

www.fluke.com

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
10.00000 V @ 1 kHz	9.999973	9.99998	9.99898	10.00096	25.0 μ V/V
19.00000 V @ 1 kHz	19.000031	18.99987	18.99837	19.00170	18.0 μ V/V
10.00000 V @ 3 kHz	9.999959	9.99979	9.99877	10.00115	25.0 μ V/V
10.00000 V @ 10 kHz	9.999924	9.99992	9.99873	10.00111	25.0 μ V/V
10.00000 V @ 30 kHz	10.000012	9.99993	9.99706	10.00296	25.0 μ V/V
10.00000 V @ 60 kHz	10.000033	10.00005	9.99208	10.00798	50.0 μ V/V
10.00000 V @ 100 kHz	9.999738	9.99980	9.99179	10.00769	80.0 μ V/V
10.00000 V @ 500 kHz	9.993887	10.02995	9.65395	10.33383	400.0 μ V/V
10.00000 V @ 1 MHz	9.989339	9.90887	9.64945	10.32923	2,500.0 μ V/V
200 V Range					
100.0000 V @ 20 Hz	99.99926	100.0001	99.9849	100.0137	50.0 μ V/V
100.0000 V @ 55 Hz	99.99864	99.9992	99.9867	100.0105	39.0 μ V/V
100.0000 V @ 300 Hz	99.99861	99.9988	99.9887	100.0085	31.0 μ V/V
1.0000 V @ 1 kHz	1.00000	1.0000	0.9975	1.0025	400.0 μ V/V
100.0000 V @ 1 kHz	99.99805	99.9980	99.9881	100.0079	35.0 μ V/V
100.0000 V @ 3 kHz	99.99745	99.9955	99.9855	100.0093	37.0 μ V/V
100.0000 V @ 10 kHz	99.99831	99.9961	99.9864	100.0102	37.0 μ V/V
100.0000 V @ 30 kHz	99.99809	99.9945	99.9686	100.0276	30.0 μ V/V
100.0000 V @ 60 kHz	99.99869	99.9982	99.9192	100.0782	40.0 μ V/V
100.0000 V @ 100 kHz	99.99684	100.0094	99.9173	100.0763	120.0 μ V/V
1000 V Range					
500.000 V @ 55 Hz	500.0063	500.008	499.918	500.094	35.0 μ V/V
500.000 V @ 300 Hz	500.0187	500.018	499.931	500.107	31.0 μ V/V
5.000 V @ 1 kHz	5.0000	5.000	4.974	5.026	400.0 μ V/V
500.000 V @ 1 kHz	500.0139	500.014	499.926	500.102	25.0 μ V/V
500.000 V @ 3 kHz	500.0032	499.997	499.915	500.091	25.0 μ V/V
500.000 V @ 10 kHz	500.0024	500.004	499.914	500.090	26.0 μ V/V
500.000 V @ 30 kHz	500.0195	500.030	499.796	500.242	90.0 μ V/V
1000.0000 V @ 55 Hz	1000.01570	999.9743	999.6847	1000.3467	31.0 μ V/V
1000.000 V @ 300 Hz	1000.0356	1000.037	999.705	1000.367	80.0 μ V/V
1000.000 V @ 1 kHz	1000.0350	1000.025	999.704	1000.366	74.0 μ V/V
1000.000 V @ 3 kHz	1000.0118	999.986	999.681	1000.343	75.0 μ V/V
1000.000 V @ 10 kHz	1000.0068	1000.016	999.676	1000.338	105.0 μ V/V
1000.000 V @ 30 kHz	1000.0551	1000.164	998.579	1001.531	310.0 μ V/V

DC Current Verification

Fluke Corporation	Telephone	Facsimile	Internet	Revision	2.19
1420 75th St SW, Everett WA 98203 USA	888.993.5853	425.446.6390	www.fluke.com		

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
200 μA Range					
100.00000 μ A	99.999661	99.99965	99.99776	100.00156	5.0 μ A/A
-100.00000 μ A	-99.999824	-99.99983	-100.00172	-99.99792	5.0 μ A/A
2 mA Range					
1.0000000 mA	0.99999671	0.9999966	0.9999777	1.0000157	4.7 μ A/A
-1.0000000 mA	-0.99999889	-0.9999991	-1.0000179	-0.9999799	4.7 μ A/A
20 mA Range					
10.000000 mA	9.9999868	9.999980	9.999787	10.000187	3.8 μ A/A
-10.000000 mA	-9.9999905	-9.999992	-10.000191	-9.999791	3.8 μ A/A
200 mA Range					
100.00000 mA	99.998961	99.99900	99.99366	100.00426	11.2 μ A/A
-100.00000 mA	-99.998893	-99.99889	-100.00419	-99.99359	11.2 μ A/A
2 A Range					
1.0000000 A	0.99999446	0.9999940	0.9997685	1.0002205	14.1 μ A/A
-1.0000000 A	-0.99998182	-0.9999798	-1.0002078	-0.9997558	14.1 μ A/A
20 A Range					
10.000000 A	10.0002345	10.000073	9.995284	10.005185	100.0 μ A/A
-10.000000 A	-10.0001236	-10.000313	-10.005074	-9.995174	100.0 μ A/A
AC Current Verification					
200 μA Range					
100.0000 μ A @ 55 Hz	100.00156	99.9967	99.9186	100.0846	100.0 μ A/A
10.0000 μ A @ 300 Hz	10.00128	9.9937	9.9714	10.0312	792.0 μ A/A
100.0000 μ A @ 300 Hz	100.00246	100.0000	99.9195	100.0855	60.0 μ A/A
100.0000 μ A @ 1 kHz	100.00185	99.9970	99.9188	100.0848	60.0 μ A/A
100.0000 μ A @ 5 kHz	99.98295	99.9925	99.9000	100.0659	194.0 μ A/A
100.0000 μ A @ 10 kHz	99.94803	99.9830	99.8651	100.0310	199.0 μ A/A
2 mA Range					
1.000000 mA @ 55 Hz	1.0000153	0.999941	0.999435	1.000595	100.0 μ A/A
0.010000 mA @ 300 Hz	0.0100013	0.009992	0.009758	0.010245	1,500.0 μ A/A
1.000000 mA @ 300 Hz	1.0000067	0.999971	0.999427	1.000587	40.0 μ A/A
1.000000 mA @ 1 kHz	0.9999909	0.999943	0.999411	1.000571	45.0 μ A/A
1.000000 mA @ 5 kHz	1.0000539	0.999930	0.999474	1.000634	65.0 μ A/A
1.000000 mA @ 10 kHz	1.0000471	0.999857	0.999467	1.000627	95.0 μ A/A
20 mA Range					
10.00000 mA @ 55 Hz	9.999992	9.99958	9.99419	10.00579	100.0 μ A/A
Fluke Corporation	Telephone	Facsimile	Internet		Revision 2.19
1420 75th St SW, Everett WA 98203 USA	888.993.5853	425.446.6390	www.fluke.com		

Certificate Number: EVL769023

Date of Calibration: 24-Jan-2022

Calibration Data

Parameter	Nominal Value	Measurement Result	Limits of Error		Expanded Uncertainty
			Lower Limit	Upper Limit	
0.10000 mA @ 300 Hz	0.100002	0.09993	0.09757	0.10244	1,400.0 μ A/A
10.00000 mA @ 300 Hz	10.000024	9.99990	9.99422	10.00582	40.0 μ A/A
10.00000 mA @ 1 kHz	9.999863	9.99969	9.99406	10.00566	40.0 μ A/A
10.00000 mA @ 5 kHz	0.81	10.00023	9.99528	10.00688	100.0 μ A/A
10.00000 mA @ 10 kHz	10.002298	10.00076	9.99650	10.00810	122.0 μ A/A
200 mA Range					
100.0000 mA @ 55 Hz	99.99897	99.9924	99.9445	100.0535	100.0 μ A/A
10.0000 mA @ 300 Hz	10.00002	9.9992	9.9730	10.0271	110.0 μ A/A
100.0000 mA @ 300 Hz	99.99902	99.9956	99.9445	100.0535	40.0 μ A/A
100.0000 mA @ 1 kHz	99.99704	99.9931	99.9425	100.0515	40.0 μ A/A
100.0000 mA @ 5 kHz	100.01532	100.0027	99.9608	100.0698	100.0 μ A/A
100.0000 mA @ 10 kHz	100.02898	100.0157	99.9745	100.0835	110.0 μ A/A
2 A Range					
1.000000 A @ 55 Hz	0.9999914	0.999912	0.999046	1.000936	100.0 μ A/A
0.100000 A @ 300 Hz	0.0999990	0.099989	0.099689	0.100310	140.0 μ A/A
1.000000 A @ 300 Hz	0.9999869	0.999946	0.999042	1.000932	50.0 μ A/A
1.000000 A @ 1 kHz	1.0000428	0.999995	0.999098	1.000988	40.0 μ A/A
1.000000 A @ 5 kHz	1.0001310	1.000267	0.999076	1.001186	210.0 μ A/A
1.000000 A @ 10 kHz	1.0004200	1.000679	0.999365	1.001475	520.0 μ A/A
20 A Range					
1.00000 A @ 300 Hz	0.999987	0.99986	0.99669	1.00329	140.0 μ A/A
10.00000 A @ 55 Hz	10.000356	9.99907	9.98896	10.01176	160.0 μ A/A
10.00000 A @ 300 Hz	10.000561	9.99938	9.98916	10.01196	120.0 μ A/A
10.00000 A @ 1 kHz	10.000921	9.99982	9.98952	10.01232	90.0 μ A/A
10.00000 A @ 5 kHz	10.001658	10.00757	9.97425	10.02906	550.0 μ A/A
10.00000 A @ 10 kHz	10.011821	10.00903	9.98439	10.03925	700.0 μ A/A
Frequency Verification					
1.000000 MHz	1.000000	1.0000030	0.9999880	1.0000120	1.3 μ Hz/Hz