

Added new
Grid views for
results of
searched
batches
25/07/2026

<

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

Batches

Search batches

Q

>

Advanced search

List of batches

☐	ID	Batch Name	Fabrication Date	Treatment	
☐	1	batch 1	01/12/2024	treatment A	
☐	2	batch 2	02/01/2025	treatment A	
☐	3	batch 3	02/02/2025	treatment A	
☐	4	batch 4	02/03/2025	treatment A	

Rows per page: 5 1-5 of 8 < >

Batch ID

Batch Name *

Description

Fabrication Date

Treatment

Project ID

Lab ID

* = Required

NEW

ADD

UPDATE

DELETE

User

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

Acquire

SETUP

RUN

Connected Equipment

Select equipment

Measurement Range

V_{start}

0

V_{stop}

1

V_{step}

0.1

+

Display Setup

X Axis

Mode

Auto

Scale

Linear

Y Axis

Mode

Auto

Scale

Linear

Stop
Button
5/5/2026

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

User ▾

Acquire


SETUP

RUN

RUN

STOP

I-V Curve

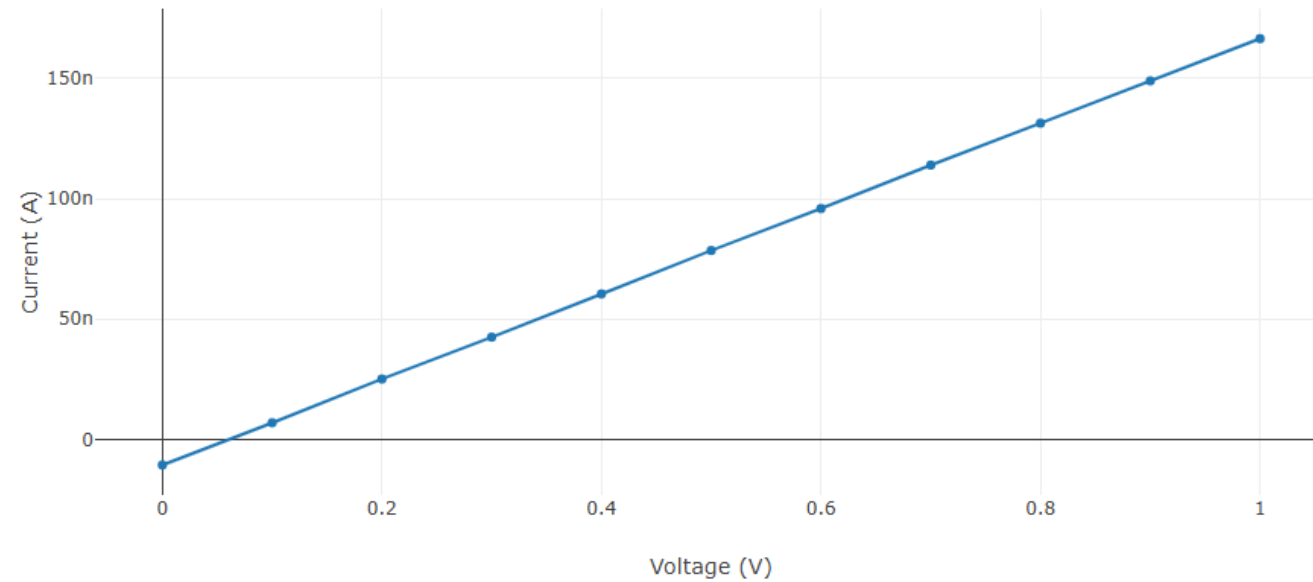

SAVE DATA TO .CSV

Save Data
To .CSV
Button
4/5/2026

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

User

Acquire


SETUP

RUN

RUN



I-V Curve

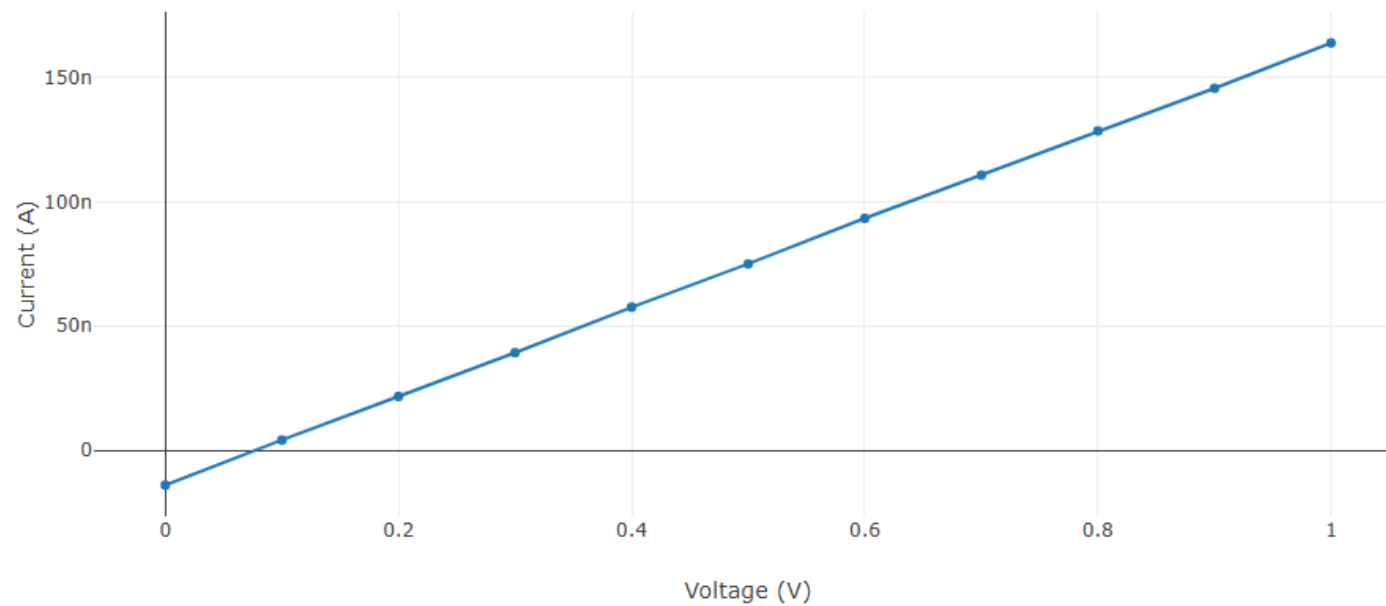

SAVE DATA TO .CSV

Dashboard

Experiment

► Acquire

⊗ Equipment

Data

■ Batches

◆ Samples

□ Files

Analysis

~ Graphs

↗ Export

Settings

○ Database

Ⓒ Users

 Chat

Acquire

SETUP

RUN

Connected Equipment

Keithley 6487 PICOAMMETER / VOLTAGE SOURCE ▾

Measurement Range

 V_{start}

0

 V_{stop}

1

 V_{step}

0.1

+

 V_{start}

0

 V_{stop}

-1

 V_{step}

0.1

-

 V_{start}

0

 V_{stop}

2

 V_{step}

0.1

-

 V_{start}

0

 V_{stop}

-2

 V_{step}

0.1

-

Display Setup

X Axis

Mode

Auto ▾

Scale

Linear ▾

Y Axis

Mode

Auto ▾

Scale

Linear ▾

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users


Chat

Acquire

SETUP

RUN

RUN

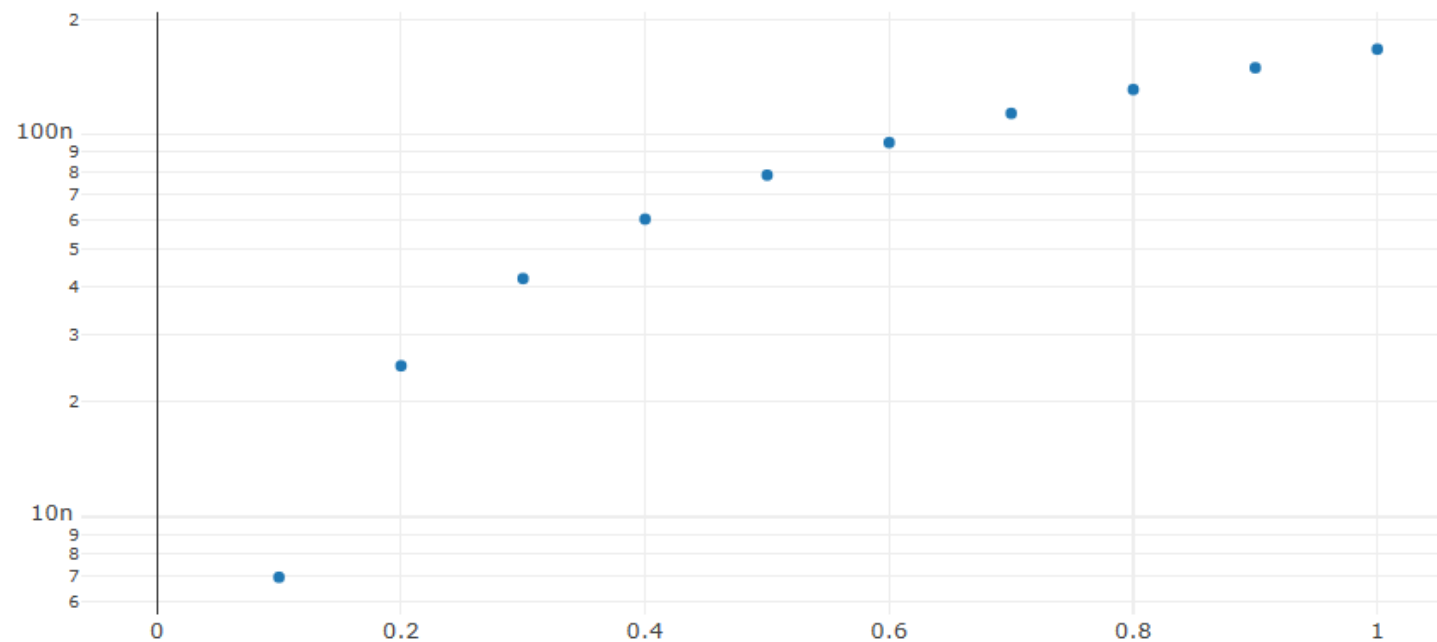

 Dashboard

Experiment

 Acquire Equipment

Data

 Batches Samples Files

Analysis

 Graphs Export

Settings

 Database Users Chat

Equipment

All

New

Keithley 2461 SourceMeter®

Keithley 2657A HIGH POWER SYSTEM SourceMeter®

Keithley 2400 SourceMeter

Keithley 6487 PICOAMMETER / VOLTAGE SOURCE

Agilent B1500A Semiconductor Device Parameter Analyzer

CONNECT EQUIPMENT

DISCONNECT EQUIPMENT

Id

4

Name

Keithley 6487 PICOAMMETER / VO

Manufacturer

Tektronix

Model

6487

Serial Number

Purchase Year

Calibration Due

dd/mm/yyyy



Location

Connecting String

GPIB0::22::INSTR

Notes

ADD

UPDATE

DELETE