

Implemented Search batch button with advanced search, 18/08/2026 database in desktop work computer

<

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

Batches

Search batches

Advanced search

ID range

from

to

Fabrication date range

from

01/01/2024

to

01/12/2024

Project Id

Lab Id

List of found batches

	ID	Batch Name	Fabrication Date	Treatment
	1	IrOxNewSM	2024-12-01	Standard tr...
	10	MBEmesfets	2024-12-01	Standard tr...
	12	IrOxNewSMAftCoat	2024-12-01	Standard tr...

Rows per page:

5

1-3 of 3

<

>

Batch ID

Batch Name *

IrOxNewSM

Description

IrOx SBDs using new milled shadow masks

Fabrication Date *

01/12/2024

Treatment

Standard treatment: Ohmic 450 C, 3min, N2, furnace.
IrOx/Ir 40/40 nm

Project ID

Lab ID

* = Required

NEW

ADD

UPDATE

DELETE

© 2026 ExpeGraph by Giang T. Dang.

Implemented Search batch button with advanced search, 18/08/2026 database in desktop work computer

<

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

User ▾

Batches

Search batches

Q

Advanced search

☒ ID range

from

1

to

20

☒ Fabrication date range

from

01/01/2024

to

18/12/2024

☐ Project Id

☐ Lab Id

List of found batches

■ ■ ■

≡

⬇

Q

☐	ID ↑	Batch Name	Fabrication Date	Treatment
☐	1	IrOxNewSM	2024-12-01	Standard tr...
☐	10	MBEmesfets	2024-12-01	Standard tr...
☐	11	NegLOBefCoat	2024-12-05	Standard tr...
☐	12	IrOxNewSMAftCoat	2024-12-01	Standard tr...
☐	13	NegLOAftCoat	2024-12-05	Standard tr...
☐	14	NewSMnewGO	2024-12-06	Standard tr...
☐	15	ThickIr	2024-12-16	Standard tr...

Rows per page: 50 ▾ 1-7 of 7 < >

Batch ID

Batch Name *

IrOxNewSM

Description

IrOx SBDs using new milled shadow masks

Fabrication Date *

01/12/2024

Treatment

Standard treatment: Ohmic 450 C, 3min, N2, furnace. IrOx/Ir 40/40 nm

Project ID

Lab ID

* = Required

NEW

ADD

UPDATE

DELETE

© 2026 ExpeGraph by Giang T. Dang.

Added new
Grid views for
results of
searched
batches
25/07/2026
Database in
Laptop
computer

<

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

Batches

Advanced search

List of batches

☐	ID	Batch Name	Fabrication Date	Treatment
☐	1	batch 1	01/12/2024	treatment A
☐	2	batch 2	02/01/2025	treatment A
☐	3	batch 3	02/02/2025	treatment A
☐	4	batch 4	02/03/2025	treatment A

Rows per page: 5 1-5 of 8

Batch ID

Batch Name *

Description

Fabrication Date

Treatment

Project ID

Lab ID

* = Required

NEW

ADD

UPDATE

DELETE

© 2026 ExpeGraph by Giang T. Dang.

Change
Icons
10/07/2026

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

Acquire

SETUP RUN

Connected Equipment

Select equipment

Measurement Range

V_{start}

0

V_{stop}

1

V_{step}

0.1

+

Display Setup

X Axis

Mode

Auto

Scale

Linear

Y Axis

Mode

Auto

Scale

Linear

Stop
Button
5/5/2026

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

User ▾

Acquire


SETUP

RUN

RUN

STOP

I-V Curve

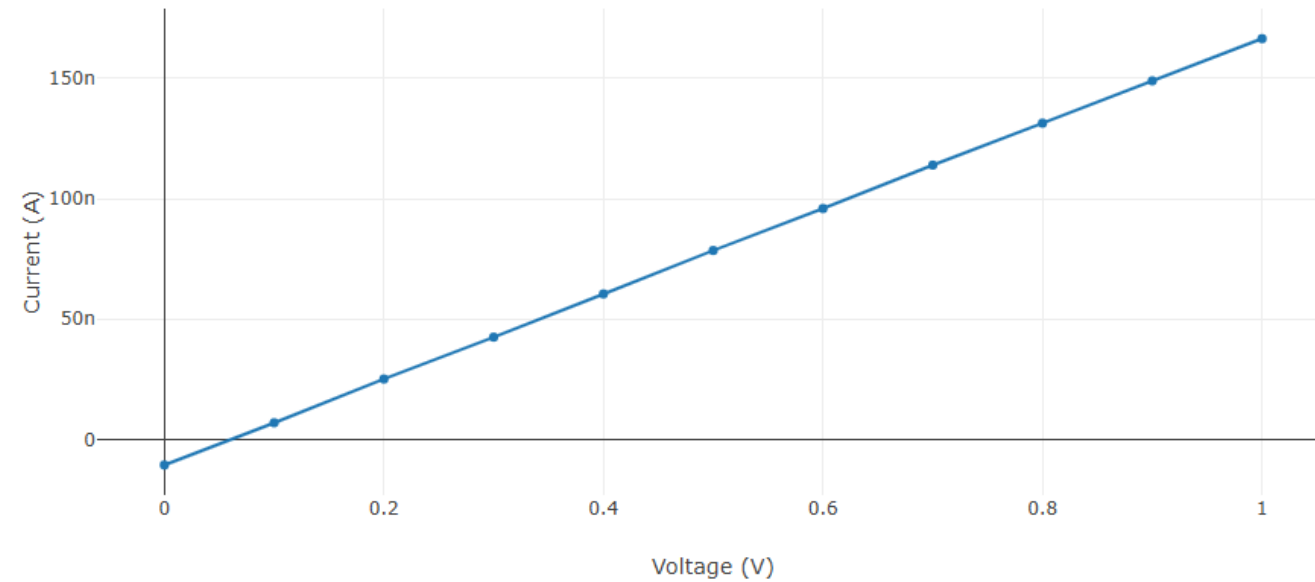

SAVE DATA TO .CSV

Save Data
To .CSV
Button
4/5/2026

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users

Chat

User

Acquire


SETUP

RUN

RUN



I-V Curve

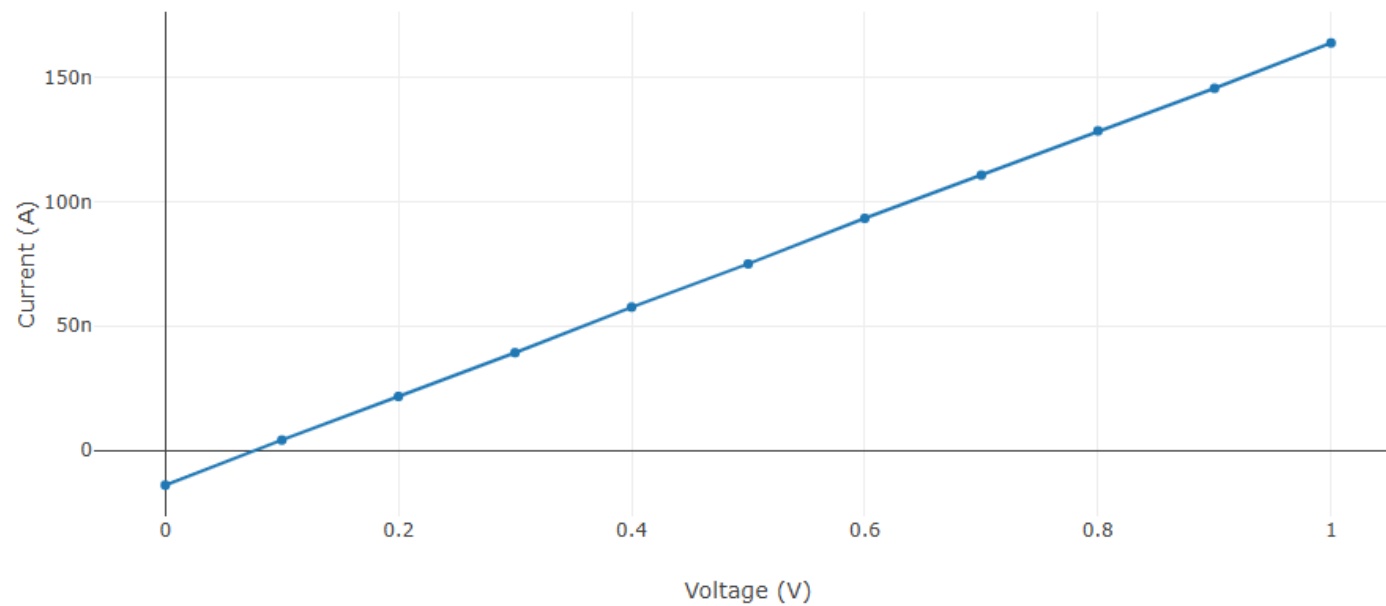

SAVE DATA TO .CSV

Dashboard

Experiment

► Acquire

⊗ Equipment

Data

■ Batches

◆ Samples

□ Files

Analysis

~ Graphs

↗ Export

Settings

○ Database

⊙ Users

 Chat

Acquire

SETUP

RUN

Connected Equipment

Keithley 6487 PICOAMMETER / VOLTAGE SOURCE ▾

Measurement Range

 V_{start}

0

 V_{stop}

1

 V_{step}

0.1

+

 V_{start}

0

 V_{stop}

-1

 V_{step}

0.1

-

 V_{start}

0

 V_{stop}

2

 V_{step}

0.1

-

 V_{start}

0

 V_{stop}

-2

 V_{step}

0.1

-

Display Setup

X Axis

Mode

Auto ▾

Scale

Linear ▾

Y Axis

Mode

Auto ▾

Scale

Linear ▾

Dashboard

Experiment

Acquire

Equipment

Data

Batches

Samples

Files

Analysis

Graphs

Export

Settings

Database

Users


Chat

Acquire

SETUP

RUN

RUN

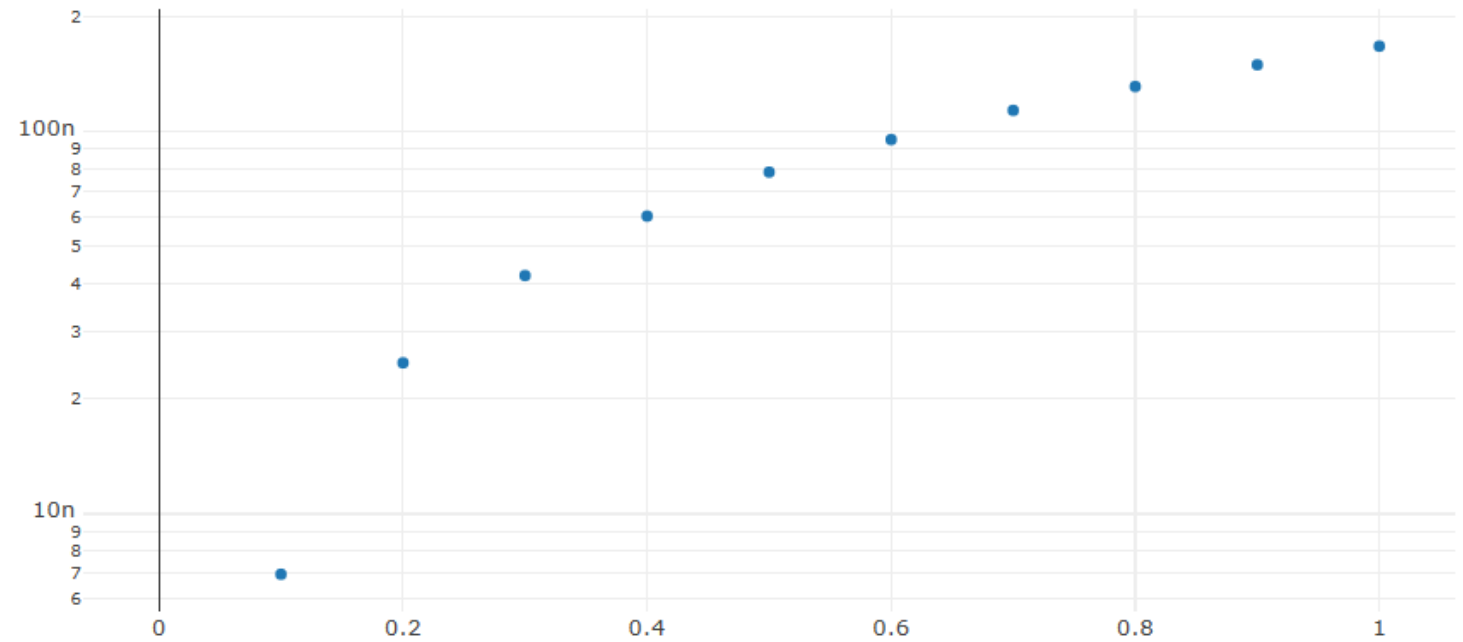

 Dashboard

Experiment

► Acquire

 Equipment

Data

 Batches

◆ Samples

□ Files

Analysis

~ Graphs

↗ Export

Settings

○ Database

◎ Users

 Chat

Equipment

All

New

Keithley 2461 SourceMeter®

Keithley 2657A HIGH POWER SYSTEM SourceMeter®

Keithley 2400 SourceMeter

Keithley 6487 PICOAMMETER / VOLTAGE SOURCE

Agilent B1500A Semiconductor Device Parameter Analyzer

CONNECT EQUIPMENT

DISCONNECT EQUIPMENT

Id

4

Name

Keithley 6487 PICOAMMETER / VO

Manufacturer

Tektronix

Model

6487

Serial Number

Purchase Year

Calibration Due

dd/mm/yyyy



Location

Connecting String

GPIB0::22::INSTR

Notes

ADD

UPDATE

DELETE