ArIso · Ar 96 % / Iso 4 % · gap 0.15 mm

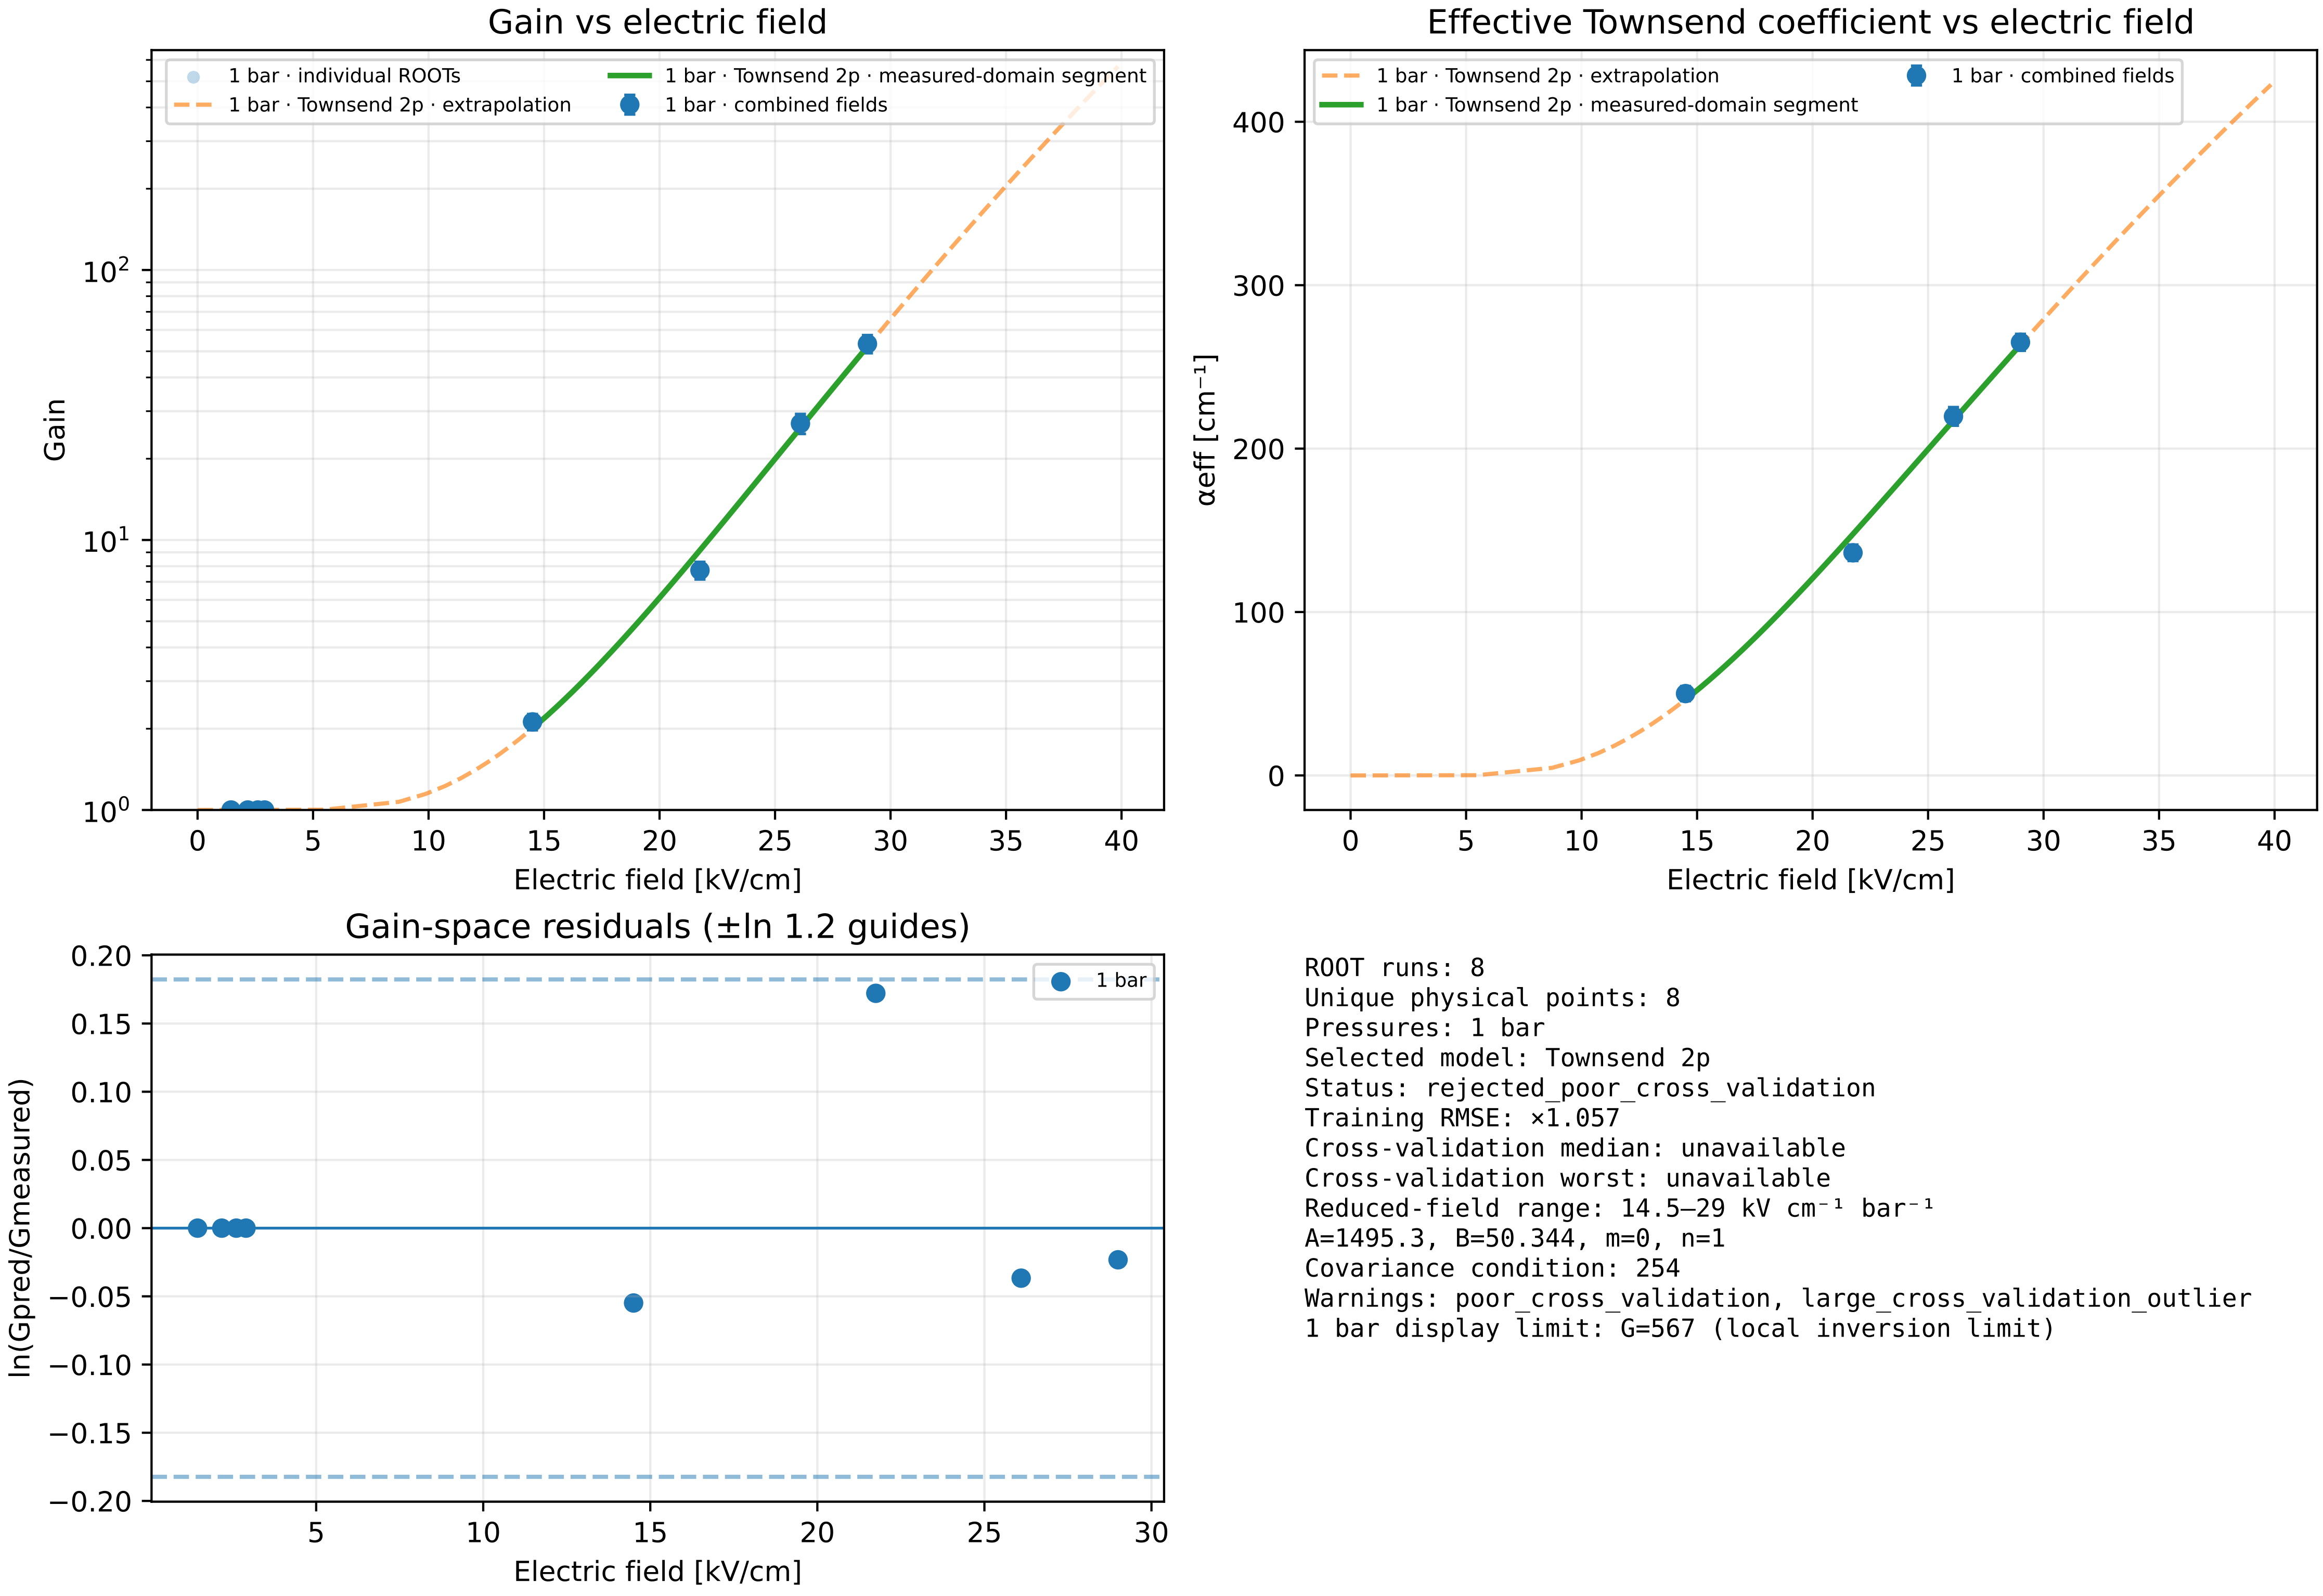


```
ROOT runs: 8
Unique physical points: 8
Pressures: 1 bar
Selected model: Townsend 2p
Status: rejected_poor_cross_validation
Training RMSE: ×1.057
Cross-validation median: unavailable
Cross-validation worst: unavailable
Reduced-field range: 14.5–29 kV cm⁻¹ bar⁻¹
A=1495.3, B=50.344, m=0, n=1
Covariance condition: 254
Warnings: poor_cross_validation, large_cross_validation_outlier
1 bar display limit: G=567 (local inversion limit)
```

Extrapolation capped at G=1e+07 or at the local model limit

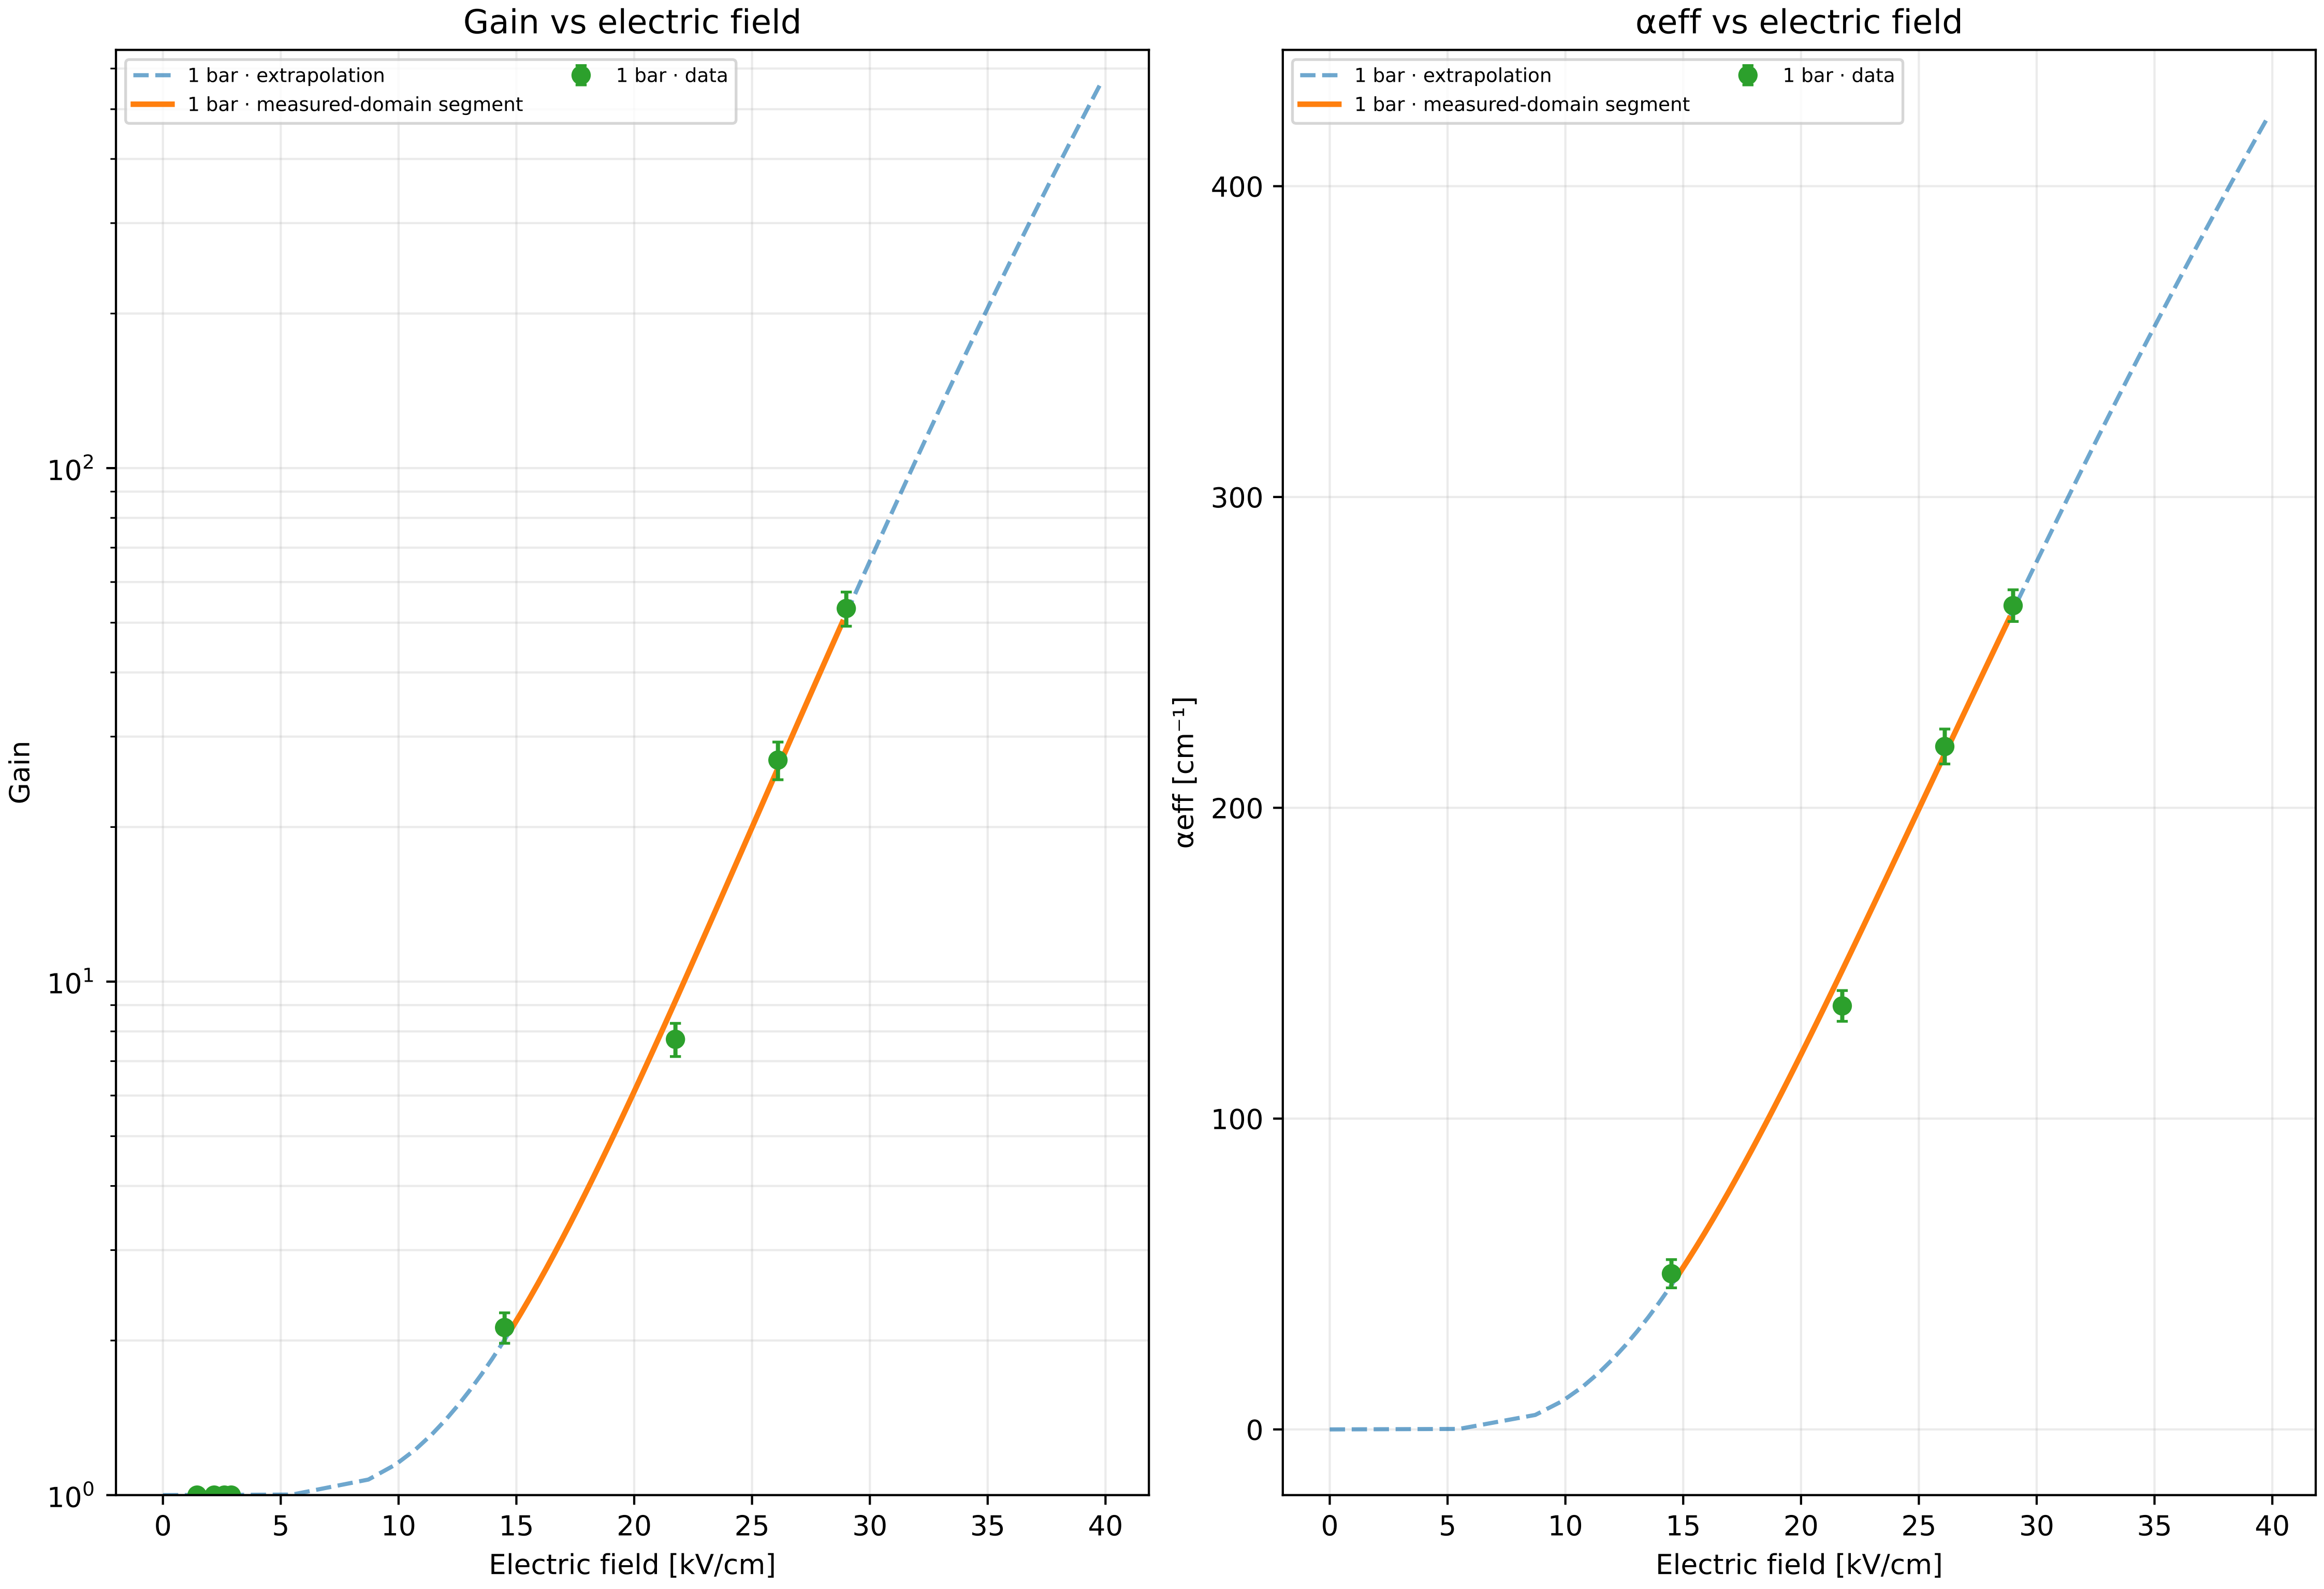

Exact combined points used by the fit · page 1/1
Repeated ROOTs at the same field are pooled once; all source ROOTs remain on disk.

p [bar]	E [kV/cm]	E/p	Gain	σGain	αeff [cm⁻¹]	npe	runs
1	1.45	1.45	1	0	—	100	1
1	2.175	2.175	1	0	—	100	1
1	2.61	2.61	1	0	—	100	1
1	2.9	2.9	1	0	—	100	1
1	14.5	14.5	2.12	0.144	50.0944	100	1
1	21.75	21.75	7.72	0.573	136.254	100	1
1	26.1	26.1	27	2.28	219.722	100	1
1	29	29	53.29	4.07	265.05	100	1

Progressive model selection
The higher-order model is selected only when new points improve out-of-sample prediction.

Candidate	k	AICc	CV median	CV worst	usable	warnings
Townsend 2p	2	-7.09	—	—	no	poor cross validation, large cross validation outlier