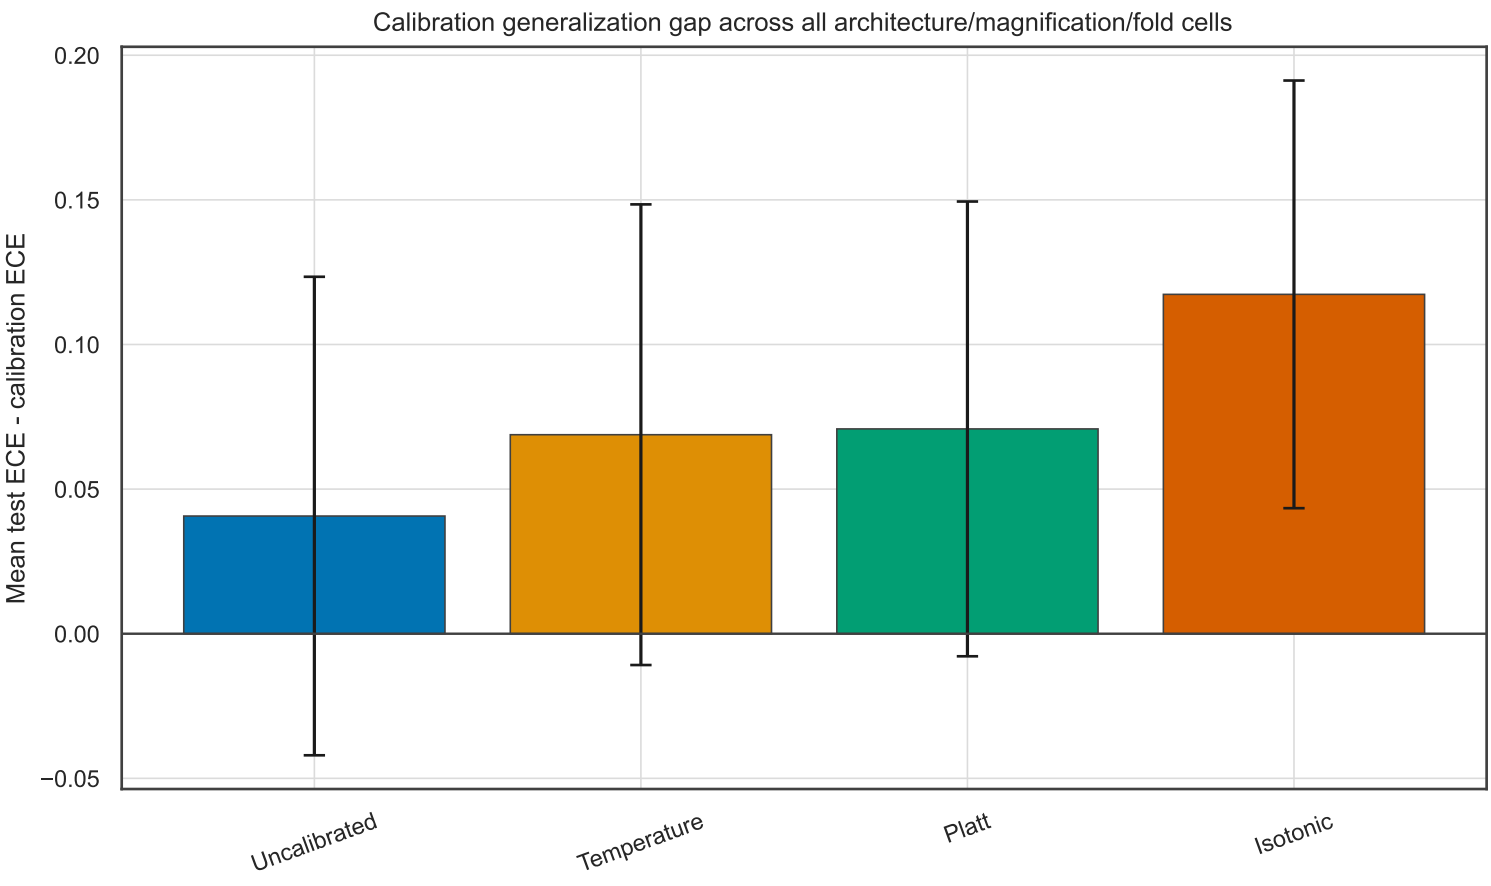
Calibration generalization gap across all architecture/magnification/fold cells
Mean test ECE - calibration ECE
0.20
0.15
0.10
0.05
0.00
−0.05
Uncalibrated
Temperature
Platt
Isotonic