NI PXI/PXIe-2527 Specifications

32 × 1 Relay Multiplexer

このドキュメントには、日本語ページも含まれています。

This document lists specifications for the NI PXI/PXIe-2527 (NI 2527) 32×1 multiplexer relay module. All specifications are subject to change without notice. Visit ni.com/manuals for the most current specifications.

Topologies1-wire 64×1 multiplexer, 1-wire dual 32×1

multiplexer, 2-wire 32 × 1 multiplexer, 2-wire dual 16 × 1 multiplexer, 4-wire 16 × 1 multiplexer, Independent

Refer to the NI Switches Help for detailed topology information.



Caution To ensure the specified EMC performance, operate this product only with shielded cables and accessories.



Caution Device relays might change state momentarily during electrostatic discharge.



Caution Refer to the *Read Me First: Safety and Electromagnetic Compatibility* document at ni.com/manuals for important safety and compliance information.

About These Specifications

Specifications characterize the warranted performance of the instrument under the stated operating conditions.

Typical Specifications are specifications met by the majority of the instrument under the stated operating conditions and are tested at 23 °C. Typical specifications are not warranted.

Input Characteristics

All input characteristics are DC, AC_{rms} , or a combination unless otherwise specified.

Maximum switching voltage

Channel-to-channel300 V
Channel-to-ground300 V, CAT I



Caution This module is rated for Measurement Category I and is intended to carry signal voltages no greater than 300 V. This module can withstand up to 1,500 V impulse voltage. Do *not* use this module for connections to signals or for measurements within Measurement Categories II, III, or IV.



Caution Do *not* connect to MAINs supply circuits (e.g., wall outlets) of 115 or 230 VAC. Refer to the *Read Me First: Safety and Electromagnetic Compatibility* document for more information about Measurement Categories.





Caution The maximum switching power is limited by the maximum switching current, the maximum voltage, and must not exceed 60 W, 62.5 VA.

Maximum switching power (per channel)






Figure 1. Maximum Switching Power for DC Loads (per channel)



Note The minimum switch load is not recommended for 2-wire resistance measurements.



Note Switching inductive loads (for example, motors and solenoids) can produce high voltage transients in excess of the module's rated voltage. Without additional protection, these transients can interfere with module operation and impact relay life. For more information about transient suppression, visit ni.com/info and enter the Info Code induct.

DC path resistance typically remains low for the life of the relay. At the end of relay life, the path resistance rapidly rises above 1 Ω . Load ratings apply to relays used within the specification before the end of relay life.

Differential thermal EMF

Typical¹......2.5 μV Maximum.....<12 μV

Channel-to-channel DC leakage.....500 GΩ @ 300 V

Bandwidth (-3 dB, 50 Ω termination)

1-wire>30 MHz 2-wire>25 MHz

Dynamic Characteristics

 Relay operate time
 1 ms

 Maximum
 3.4 ms



Note Certain applications may require additional time for proper settling. Refer to the *NI Switches Help* for information about including additional settling time.



Note The relays used in the NI 2527 are field replaceable. Refer to the *NI Switches Help* for information about replacing a failed relay.

Trigger Characteristics

Input trigger

SourcesPXI trigger lines 0–7
Minimum pulse width150 ns



Note The NI 2527 recognizes trigger pulse widths less than 150 ns when you disable digital filtering. Refer to the *NI Switches Help* for information about disabling digital filtering.

¹ To ensure the typical thermal EMF, power down all relays and avoid pulsing high currents near the channels you are measuring. For more information about powering down latching relays, refer to the Power Down Latching Relays After Debounce property in NI-SWITCH or the Power Down Latching Relays After Settling property in NI-DAQmx.

Output trigger

Destinations	PXI trigger lines 0-7
Pulse width	Programmable
	(1 μs to 62 μs)

Thermocouple Measurement

You can use the NI 2527 and the NI TB-2627 to measure thermocouples. NI software can convert a thermocouple voltage to the thermocouple temperature. For example code, visit ni.com/zone, click the Example Code link in the navigation bar, and enter PXI-2527 in the Search field.

When measuring thermocouples, be sure to account for error in your measurements. The total error in thermocouple measurement is the sum of the system error (determined by the thermal EMF of the NI 2527 and the CJC temperature of the NI TB-2627) and the thermocouple error (determined by the type of thermocouple used).

Determining the System Error

To determine the system error for the NI 2527/TB-2627, first calculate the error due to thermal EMF of the NI 2527 using the following equation.

$$E_{EMF} = \left(\frac{T_{+I} - T}{V_{+J} - V}\right) (V_{EMF})^{1} \tag{1}$$

where

 E_{EMF} = error due to thermal EMF of the NI 2527 T = temperature being measured, in degrees Celsius $T_{+I} = T + 1$ °C V = voltage that corresponds to T V_{+I} = voltage that corresponds to T_{+I}

 V_{EMF} = thermal EMF of the NI 2527²

After you have determined the error due to thermal EMF, calculate the system error using the following equation.

$$E_S = E_{EMF} + E_{CJC} \tag{2}$$

where

 E_S = system error of the NI 2527/TB-2627 E_{EMF} = error due to thermal EMF of the NI 2527 E_{CJC} = error due to CJC temperature sensor of the NI TB-2627³

Example

Measuring a K-type thermocouple at 200 °C with a CJC temperature of 25 °C, the system error of the NI 2527/TB-2627 is calculated below.⁴

Assuming typical thermal EMF (2.5 μV), first calculate the error due to thermal EMF using Equation 1.

$$E_{EMF} = \left(\frac{201 \text{ °C} - 200 \text{ °C}}{8.178 \text{ mV} - 8.138 \text{ mV}}\right) (0.0025 \text{ mV})$$

To determine the system error, add the error due to thermal EMF to the error due to the CJC temperature sensor using Equation 2.

$$E_S = 0.063 \, ^{\circ}\text{C} + 0.5 \, ^{\circ}\text{C}$$

= 0.563 $^{\circ}\text{C}$

Determining the Thermocouple Error

Independent of the NI 2527/TB-2627 system, thermocouple error is the greater of the following values: $\pm a$ temperature range or $\pm a$ percent of the measurement.

In the example, a standard grade K-type thermocouple is used to measure 200 °C. The error for a standard grade K-type thermocouple is ± 2.2 °C $or \pm 0.75\%$ of the measurement temperature. Escause $\pm 0.75\%$ of 200 °C (± 1.5 °C) is less than ± 2.2 °C, the error of a standard grade K-type thermocouple is ± 2.2 °C.

¹ In thermocouple reference tables, T and T_{+I} are known values used to calculate the slope of the thermocouple Temperature vs. Voltage graph. Refer to a thermocouple reference table to determine the values of V and V_{+I} that correspond to T and T_{+I} , respectively.

² Refer to the *Input Characteristics* section of this document to determine the thermal EMF value of the NI 2527. For optimal thermocouple measurement performance ($V_{EMF} = 2.5 \,\mu\text{V}$), power down the latching relays of the NI 2527. For more information about powering down latching relays, refer to the Power Down Latching Relays After Debounce property in NI-SWITCH or the Power Down Latching Relays After Settling property in NI-DAQmx.

³ From 15 °C to 35 °C, the NI TB-2627 has an accuracy of ±0.5 °C. From 0 °C to 15 °C and 35 °C to 55 °C, the NI TB-2627 has an accuracy of ±1.0 °C. For more information about temperature sensor accuracy, refer to the *NI TB-2627 Installation Instructions*.

In this example, the values of V and V_{+J} are found in the thermocouple reference tables of Omega Engineering's The Temperature Handbook. Vol. 29. Stamford, CT: Omega Engineering Inc, 1995.

⁵ Omega Engineering. The Temperature Handbook. Vol. 29. Stamford, CT: Omega Engineering Inc, 1995.

Determining the Total Error

The total error in thermocouple measurement is the sum of the system error and the thermocouple error. Use the following equation to determine the total error in thermocouple measurement.

$$E_T = E_S + E_{Th} \tag{3}$$

where E_T = total error in thermocouple measurement E_S = system error

 E_{Th} = thermocouple error

To determine the total error in thermocouple measurement in the example, add the thermocouple error to the system error using Equation 3, as illustrated below.

$$E_T = 0.56 \, ^{\circ}\text{C} + 2.2 \, ^{\circ}\text{C}$$

Assuming typical thermal EMF, the total error in thermocouple measurement at 200 °C for the NI 2527/TB-2627 with a K-type thermocouple is ±2.76 °C.

Physical Characteristics

i ilyoloai ollaraotoriotio	U
Relay type	.Electromechanical, latching
Relay contact material	.Palladium-ruthenium, gold covered
I/O connector	.100 position HDI right angle, male
Power requirement	
PXI	.6 W at 5 V,
	2.5 W at 3.3 V
PXI Express	.7.5 W at 12V,
•	2.5 W at 3.3 V
Dimensions $(L \times W \times H)$.3U, one slot,
	PXI/cPCI module,
	PXIe compatible
	$21.6 \times 2.0 \times 13.0 \text{ cm}$
	$(8.5 \times 0.8 \times 5.1 \text{ in.})$
Weight	209 g (7.4 oz)

Environment

Operating temperature 0 °C to 55 °C



Caution If you are using the NI 2527 with the NI PXI-101x or the NI PXI-1000B chassis, the operating temperature for the NI 2527 is 0 °C to 45 °C. Do not operate the NI 2527 above the maximum operating temperature of the chassis.

Storage temperature	.–20 °C to 70 °C
Relative humidity	.5% to 85%, noncondensing
Pollution Degree	. 2
Maximum altitude	. 2,000 m
Indoor use only.	

Shock and Vibration	
Operational Shock	30 g peak, half-sine, 11 ms pulse (Tested in accordance with IEC 60068-2-27. Test profile developed in accordance with MIL-PRF-28800F.)
Random Vibration	
Operating	5 to 500 Hz, 0.3 g_{rms}
Nonoperating	5 to 500 Hz, 2.4 g _{rms} (Tested in accordance with IEC 60068-2-64. Nonoperating test profile exceeds the requirements of MIL-PRF-28800F, Class 3.)

Diagrams

Figure 2 shows the NI 2527 power-on state.

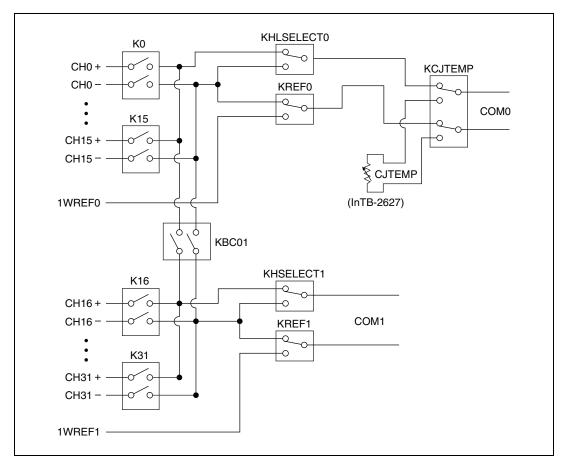


Figure 2. NI 2527 Power-On State

Figure 3 shows the NI PXI-2527 connector pinout.

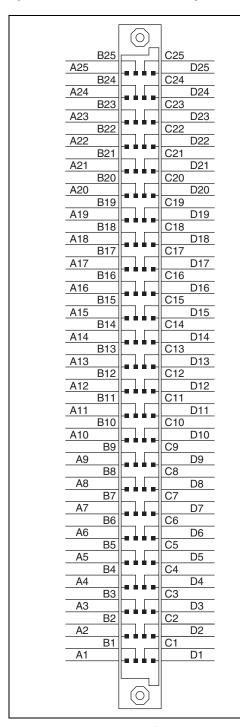


Figure 3. NI PXI-2527 Connector Pinout



Note For topology-specific connection information, refer to your device in the *NI Switches Help* and the installation instructions for any associated cables or terminal blocks.

Accessories

Visit ni.com for more information about NI accessories.

Table 1. Accessories for the NI 2527

Accessory	Manufacturer	Part Number
NI TB-2627 terminal block	NI	779358-01
IM42PGR relay replacement kit	NI	782051-01
100-pin HDI right angle mating connector*	NI	779311-01
Mating front panel connector, vertical*	AMP	5533285-1
Mating front panel connector, right-angle*	AMP	5532903-2

^{*} PCB mount, additional cover or enclosure required. See the previous safety caution.



Caution You *must* install mating connectors according to local safety codes and standards and according to the specifications provided by the connector manufacturer. You are responsible for verifying safety compliance of third-party connectors and their usage according to the relevant standard(s), including UL and CSA in North America and IEC and VDE in Europe.

Compliance and Certifications

Safety

This product meets the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1



Note For UL and other safety certifications, refer to the product label or the *Online Product Certification* section.

Electromagnetic Compatibility

This product meets the requirements of the following EMC standards for electrical equipment for measurement, control, and laboratory use:

- EN 61326-1 (IEC 61326-1): Class A emissions; Basic immunity
- EN 55011 (CISPR 11): Group 1, Class A emissions
- AS/NZS CISPR 11: Group 1, Class A emissions
- FCC 47 CFR Part 15B: Class A emissions
- ICES-001: Class A emissions



Note In the United States (per FCC 47 CFR), Class A equipment is intended for use in commercial, light-industrial, and heavy-industrial locations. In Europe, Canada, Australia and New Zealand (per CISPR 11) Class A equipment is intended for use only in heavy-industrial locations.



Note Group 1 equipment (per CISPR 11) is any industrial, scientific, or medical equipment that does not intentionally generates radio frequency energy for the treatment of material or inspection/analysis purposes.



Note For EMC declarations and certifications, refer to the *Online Product Certification* section.

CE Compliance \subset \in

This product meets the essential requirements of applicable European Directives as follows:

- 2006/95/EC; Low-Voltage Directive (safety)
- 2004/108/EC; Electromagnetic Compatibility Directive (EMC)

Online Product Certification

To obtain product certifications and the Declaration of Conformity (DoC) for this product, visit ni.com/certification, search by model number or product line, and click the appropriate link in the Certification column.

Environmental Management

NI is committed to designing and manufacturing products in an environmentally responsible manner. NI recognizes that eliminating certain hazardous substances from our products is beneficial to the environment and to NI customers.

For additional environmental information, refer to the *NI* and the Environment Web page at ni.com/environment. This page contains the environmental regulations and directives with which NI complies, as well as other environmental information not included in this document.

Waste Electrical and Electronic Equipment (WEEE)



EU Customers At the end of the product life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers, National Instruments WEEE initiatives, and compliance with WEEE Directive 2002/96/EC on Waste Electrical and Electronic Equipment, visit ni.com/environment/weee.

电子信息产品污染控制管理办法 (中国 RoHS)



中国客户 National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于National Instruments 中国 RoHS 合规性信息,请登录 ni.com/environment/rohs_china。(For information about China RoHS compliance, go to ni.com/environment/rohs_china,)



NI PXI/PXIe-2527 仕様

32×1リレーマルチプレクサ

このドキュメントには、NI PXI/PXIe-2527 (NI 2527) 32×1 マルチプレクサリレーモジュールの仕様が記載されています。すべての仕様は事前の通知なしに変更されることがあります。最新の仕様については、ni.com/manuals を参照してください。

トポロジ......単線式 64×1 マルチ プレクサ、

2 バンク単線式 32 ×1 2 バンク単線式 32 ×1 2 線式 32 ×1 マルチプ レクサ、 2 バンク 2 線式 16 ×1 マルチプレクサ、 4 線式 16 ×1 マルチプ レクサ、独立

トポロジ情報については、『NI スイッチヘルプ』を参照 してください。



注意 指定された EMC のパフォーマンスを 確保するには、シールドケーブルおよびアク セサリを必ず使用してください。



注意 デバイスリレーは、静電放電時に状態が一瞬変化する場合があります。



注意 安全規格の詳細については、ni.com/manuals から『はじめにお読みください:安全対策と電磁両立性について』を参照してください。

仕様値について

「仕様」は、記載された動作条件下で保証される計測器 の性能を示します。

「標準仕様」は、記載された動作条件下で大多数の計測 器が満たす仕様を示し、23℃で検証されています。 標準仕様は保証されている値ではありません。

入力特性

すべての入力特性は特に注釈のない限り、DC、AC_{rms}、もしくはその組み合わせとします。

最大スイッチ電圧

チャンネル間......300 V チャンネル / グランド間.......300 V、CATI



注意 このデバイスは、Measurement Category I に定格であり、使用できる信号電圧は300 V 以下です。また、1,500 V までのインパルス電圧に耐性があります。Category II、III、または IV の信号を、このモジュールに接続したり測定しないでください。



注意 115 または 230 VAC のコンセントを使用する電源回路(例:壁コンセント)に接続しないでください。測定カテゴリの詳細については、『はじめにお読みください:安全対策と電磁両立性について』を参照してください。



注意 危険電圧 (> $42.4 \text{ V}_{pk}/60 \text{ VDC}$) がリレー端子に接続されている場合、安全低電圧 ($\leq 42.4 \text{ V}_{pk}/60 \text{ VDC}$) をその他のリレー端子 に接続することはできません。



注意 最大スイッチ電力は、最大スイッチ電流と最大電圧によって制限されます。60 W、62.5 VA を超えないように注意してください。

最大スイッチ電力(チャンネルあたり)






図 1 DC 負荷に対する最大スイッチ電力 (チャンネルあたり)

最大総電流 (スイッチまたは許容)......2 A

最小スイッチ負荷20 mV/1 mA



メモ 最小スイッチ負荷は、2線式抵抗測定には推奨されていません。



メモ 誘導性負荷(モーターおよびソレノイド)を切り替えることで、モジュールの定格電圧を超える高電圧過渡信号が生じます。追加の保護を施さない場合、これらの過渡によってモジュール動作が干渉され、リレー寿命に影響を与えます。過渡減衰についての詳細は、ni.com/jp/infoで Info Code のフィールドに「jpf8kh」と入力します。

DC パス抵抗

初期	<1Ω
寿命末期	≥2 Ω

通常、DCパス抵抗は、リレーの寿命が続く間小さい値を保持します。リレーの寿命末期時には、パスの抵抗は急速に大きくなり、1Ω以上になります。負荷定格は寿命末期以前の仕様範囲内で使用されるリレーに適用されます。

接触電位 (差動)

標準値 ¹	.2.5 µV
最大値	.<12 µV

チャンネル間 DC 漏れ......500 GΩ (300 V 時)

帯域幅(-3 dB、50 Ω

2 線式>25 MHz
チャンネル間絶縁(50 Ω 終端) (単線式および 2 線式)
10 kHz>80 dB
100 kHz>60 dB

1 MHz.....>40 dB

単線式......>30 MHz

オープンチャンネル絶縁 (50 Ω 終端) (単線式および 2 線式)

10 kHz	>80	dB
100 kHz	>60	dB
1 N 41 I-	- 10	-ID

動特性

リレー動作(セット)時間

標準値	l ms	3
最大 :	3 4 r	ns



メモ アプリケーションによっては、より長い整定時間が必要な場合があります。整定時間の追加についての情報は、『NI スイッチへルプ』を参照してください。

リレー寿命

機械的	1	X	10°	サイ	(ク	ル
電気的						

300 VDC.

60 mADO	乙抵抗	5×10 ⁵ サイクル
30 VDC	2 ADC 抵抗	1 × 10 ⁵ サイクル
<30 mV.	<10 mA	25×106サイクル



メモ NI 2527 で使用されているリレーは、現場交換が可能です。破損したリレーの交換についての情報は、『NI スイッチヘルプ』を参照してください。

トリガ特性

入力トリガ

入力元	PXI 0 \sim	
最小パルス幅	150	ns

¹ 標準接触電位を得るために、すべてのリレーの電源を切り、測定しているチャンネルの周辺に高電流が流れないようにします。ラッチ型リレーの電源の切り方についての情報は、NI-SWITCHの「デバウンス後ラッチリレーの電源を切る」のプロパティまたは NI-DAQmx の「整定後ラッチリレーパワーダウン」のプロパティを参照してください。



メモ NI 2527 は、デジタルフィルタを無効にするときに、150 ns 未満のトリガパルス幅を認識することができます。デジタルフィルタを無効にする方法については、『NI スイッチヘルプ』を参照してください。

熱電対測定

NI 2527 と NI TB-2627 を使用して熱電対の測定を行うことができます。NI のソフトウェアを使用して熱電対からの電圧を温度に変換することができます。サンプルプログラムを入手するには、ni.com/zone にアクセスして、ナビゲーションバーにある「サンプル」のリンクをクリックします。検索フィールドに PXI-2527 と入力します。

熱電対を測定するときには、測定エラーを考慮する必要があります。熱電対測定の誤差は、システム誤差 (NI 2527 の接触電位と NI TB-2627 の CJC (冷接点補償) 温度による)と熱電対誤差 (使用する熱電対のタイプによる)を合わせたものです。

システム誤差を計算する

NI 2527/TB-2627 のシステム誤差を得るには、まず次の等式を使って NI 2527 の接触電位による誤差を計算します。

$$E_{EMF} = \left(\frac{T_{+1} - T}{V_{+1} - V}\right) \left(V_{EMF}\right)^{1}$$

 E_{EMF} = NI 2527 の接触電位による誤差 T = 測定された温度(摂氏) T_{+1} = T + 1 $^{\circ}$ V = T に対応する電圧

 $V_{+1} = T_{+1}$ に対応する電圧 $V_{EME} = NI \ 2527 \ の接触電位²$

接触電位による誤差を確認した後、次の等式を使用してシステム誤差を計算します。

$$E_{S} = E_{EMF} + E_{CJC} \tag{2}$$

 E_S = NI 2527/TB-2627 のシステム誤差 E_{EMF} = NI 2527 の接触電位による誤差 E_{CJC} = NI TB-2627 の CJC 温度センサによる 誤 ± 3

個

K タイプ熱電対を 200 ℂで測定する場合(CJC 温度は 25 ℂ)、NI 2527/TB-2627 のシステム誤差は次のように 計算します。 4

接触電位を標準(2.5 µV)と想定して、まず、等式 1 を使って接触電位による誤差を計算します。

$$E_{EMF} = \left(\frac{201 \text{ °C-} 200 \text{ °C}}{8.178 \text{ mV} - 8.138 \text{ mV}}\right) (0.0025 \text{ mV})$$

= 0.063 °C

システム誤差は、等式 2を使って接触電位による誤差 値を CJC 温度センサによる誤差値に加えることで得る ことができます。

$$E_S = 0.063 \text{ }^{\circ}\text{C} + 0.5 \text{ }^{\circ}\text{C}$$

= 0.563 °C

熱電対誤差を測定する

(1) NI 2527/TB-2627 システムとは関係なく、熱電対誤差は±温度範囲または±測定の割合の大きいほうの値となります。

この例では、200 \mathbb{C} の測定に標準レベルの K タイプ熱電対が使われています。この熱電対の誤差は、 ± 2.2 \mathbb{C} または 測定温度の $\pm 0.75\%$ です。 5 200 \mathbb{C} (± 1.5 \mathbb{C}) の

¹ 熱電対基準表の $T \succeq T_{+1}$ は、熱電対の温度に対する電圧のグラフでの傾斜計算に使われる値です。熱電対基準表を参照して、 $T \succeq T_{+1}$ に対応する $V \succeq V_{+1}$ の値を確認します。

² このドキュメントの「入力特性」セクションを参照して、NI 2527 の接触電位を確認します。熱電対の測定 (V_{EMF} = 2.5 μV) を最適化するには、NI 2527 のラッチ型リレーの電源を切ります。ラッチ型リレーの電源の切り方についての情報は、NI-SWITCH の「デバウンス後ラッチリレー電源切断」のプロパティまたは NI-DAQmx の「整定後ラッチリレーパワーダウン」のプロパティを参照してください。

^{3 15~35 ℃}では、NITB-2627 の確度は±0.5 ℃です。また、0~15 ℃および 35~55 ℃では、±1.0 ℃です。温度センサの確度についての詳細は、『NITB-2627 取り付け手順』を参照してください。

⁴ この例では、Vの値と V_{+1} の値は、Omega Engineering の『The Temperature Handbook』、Vol. 29. (Stamford, CT: Omega Engineering Inc, 1995) の熱電対基準表に記載されています。

Omega Engineering. The Temperature Handbook. Vol. 29. (Stamford, CT: Omega Engineering Inc, 1995)

±0.75% は、±2.2 ℃より小さい値であるため、標準レベルの K タイプ熱電対の誤差は ±2.2 ℃ということになります。

総合誤差を計算する

熱電対測定における総合誤差は、システム誤差と熱電 対誤差を足した値です。熱電対測定の総合誤差の計算に は次の式を使用します。

$$E_T = E_S + E_{Th} \tag{3}$$

 E_T = 熱電対測定の総合誤差 E_S = システム誤差 E_{Th} = 熱電対誤差

この例での熱電対測定における総合誤差を計算するに は、下記に示されているように等式 3を使用して、熱 電対誤差をシステム誤差に足します。

$$E_T = 0.56 \,^{\circ}\text{C} + 2.2 \,^{\circ}\text{C}$$

= 2.76 °C

接触電位を標準と想定すると、NI 2527/TB-2627 を K タイプ熱電対を使用して 200 $\mathbb C$ で測定した熱電対の総合誤差は $\pm 2.76 \mathbb C$ となります。

物理特性

12) 14 14 14 14 14 14 14 14 14 14 14 14 14	
リレータイプ	. メカニカル、ラッチ型
リレー接触部材質	. パラジウム / ルテニウ ム、金メッキ
I/O コネクタ	. 100 ピン HDI 直角マウ ント、オス
所要電力	
PXI Express	2.5 W(3.3 V 時)
外形寸法(奥行×幅×高さ)	3U、1 スロット、 PXI/cPCI モジュール、 PXIe 互換 21.6×2.0×13.0 cm (8.5×0.8×5.1 in.)

重量......209 g (7.4 oz)

環境

動作温度......0~55℃



注意 NI 2527 を NI PXI-101x または NI PXI-1000B シャーシで使用している場合、NI 2527 の動作温度は $0\sim45$ $^{\circ}$ です。シャーシの最高動作温度を超えた状態で NI 2527 を使用しないでください。

保管温度	−20 ~ 70 ℃
相対湿度	5 ~ 85% (結露なきこと)
汚染度	2
最大使用高度	2,000 m
室内使用のみ。	

耐衝撃 / 振動	
動作時衝擊	. 最大 30 g(半正弦 波)、11 ms パルス (IEC 60068-2-27 に準 拠して試験済み。 MIL-PRF-28800F に準 拠してテストプロファ イルを確立。)
ランダム振動	
動作時 非動作時	Julia



図 2は、電源投入状態の NI 2527 を示しています。

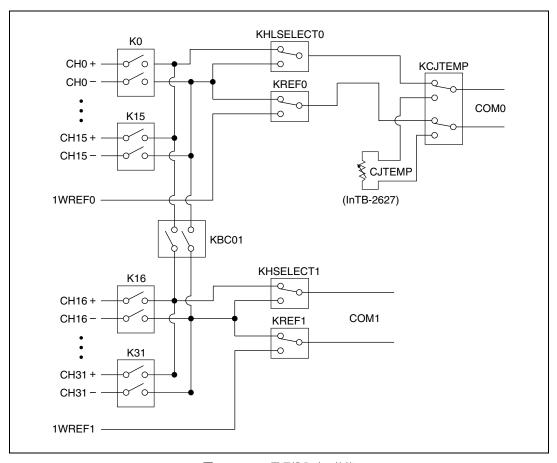


図 2 NI 2527 電源投入時の状態

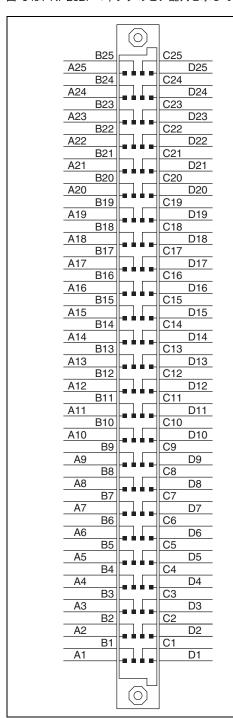


図 3 NI PXI-2527 コネクタのピン配列



メモ 各トポロジ特有の接続方法については、 『NI スイッチヘルプ』でご使用のデバイスト ピックから関連ケーブルおよび端子台の取り 付け手順を参照してください。

アクセサリ

NIアクセサリの詳細については、ni.com/jp にアクセスしてください。

表 1 NI 2527 対応のアクセサリ

アクセサリ	製造元	製品番号
NI TB-2627 端子台	NI	779358-01
IM42PGR リレー 交換キット	NI	782051-01
100 ピン HDI 直角 マウントメイトコ ネクタ *	NI	779311-01
フロントパネル用 メイトコネクタ、 垂直マウント *	AMP	5533285-1
フロントパネル用 メイトコネクタ、 直角マウント *	AMP	5532903-2

* PCB マウント、追加のカバーまたはケースが必要です。前述の安全に関する注意事項を参照してください。



注意 メイトコネクタは、必ず地域の安全 コードと基準、およびコネクタの製造元に よって提供された規格に従って取り付ける必 要があります。他社製コネクタの安全適合指 令、また該当する基準(北米では UL および CSA、ヨーロッパでは IEC および VDE を含 む)に従った使用方法を確認してください。

認可および準拠

安全性

この製品は、計測、制御、実験に使用される電気装置 に関する以下の規格および安全性の必要条件を満たし ます。

- IEC 61010-1、EN 61010-1
- UL 61010-1、CSA 61010-1



メモ UL およびその他の安全保証については、製品ラベルまたは「オンライン製品認証」セクションを参照してください。

電磁両立性

この製品は、計測、制御、実験に使用される電気装置 に関する以下の EMC 規格の必要条件を満たします。

- EN 61326-1 (IEC 61326-1): Class A エミッション、 基本イミュニティ
- EN 55011 (CISPR 11): Group 1、Class A エミッション
- AS/NZS CISPR 11: Group 1、Class A エミッション
- FCC 47 CFR Part 15B: Class A エミッション
- ICES-001: Class A エミッション



メモ 米国では(FCC 47 CFR に従って)、 Class A 機器は商業、軽工業、および重工業 の設備内での使用を目的としています。欧州、 カナダ、オーストラリア、およびニュージー ランドでは(CISPR 11 に従って)、Class A 機 器は重工業の設備内のみでの使用を目的とし ています。



メモ Group 1 機器とは (CISPR 11 に従って) 材料の処理または検査 / 分析の目的で無線周波数エネルギーを意図的に生成しない工業用、科学、または医療向け機器のことです。



メモ EMC 宣言および認証については、 「オンライン製品認証」セクションを参照して ください。

CEマーク準拠((

この製品は、該当する EC 理事会指令による基本的要件に適合しています。

- 2006/95/EC、低電圧指令(安全性)
- 2004/108/EC、電磁両立性指令(EMC)

オンライン製品認証

この製品の製品認証および適合宣言(DoC)を入手するには、ni.com/certification(英語)にアクセスして型番または製品ラインで検索し、保証の欄の該当するリンクをクリックしてください。

環境管理

ナショナルインスツルメンツは、環境に優しい製品の設計および製造に努めています。NIは、製品から特定の有害物質を除外することが、環境および NI のお客様にとって有益であると考えています。

環境の詳細な情報については、ni.com/environment (英語) の NI and the Environment (英語) を参照してください。このページには、ナショナルインスツルメンツが準拠する環境規制および指令、およびこのドキュメントに含まれていないその他の環境に関する情報が記載されています。

廃電気電子機器(WEEE)



欧州のお客様へ 製品寿命を過ぎたすべての製品は、必ずWEEE リサイクルセンターへ送付してください。WEEE リサイクルセンターおよびナショナルインスツルメンツのWEEEへの取り組み、および廃電気電子機器のWEEE 指令 2002/96/EC 準拠については、ni.com/environment/weee(英語)を参照してください。

电子信息产品污染控制管理办法 (中国 RoHS)



中国客户 National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于 National Instruments 中国 RoHS 合规性信息,请登录 ni.com/environment/rohs_china。 (For information about China RoHS compliance, go to ni.com/environment/rohs_china.)

LabVIEW. National Instruments. NI. ni.com、National Instruments のコーボレートロゴ及びイーグルロゴは、National Instruments Corporation の商標です。その他の National Instruments の商標については、ni.com/trademarks に掲載されている「Irademark Information」をご覧下さい。本文書中に記載されたその他の製品名および企業名は、それぞれの企業の商標または商号です。National Instruments の製品 / 技術を保護する特許については、ソフトウェアで参照できる特許情報(ペ**ルノー特件権)**、メディアに含まれている patents . txt ファイル。または「Notional Instruments Patent Notice」(ni.com/patents)のうち、該当するリソースから参照してください。ナショナルインスツルメンツの輸出関連法規遵守に対する方針について、また必要な HTS コード、ECCN、その他のインボート/エクスポートデータを取得する方法については、「輸出関連法規の遵守に関する情報」(ni.com/legal/export-compliance)を参照してください。