



DIAGNOSTIC
SOLUTIONS
INTERNATIONAL LLC

Certificate of Calibration

Certificate: +125177
RMA# 250022
Date Calibrated 3/6/2025
Due Date 3/6/2026

Manufacturer

Honeywell / Chadwick Helmuth

Model

VXP (Carry-On)

Calibration Interval

12 months

Part Number

901-15160-2

Type

Acquisition Unit

If any readings appear below, they are randomly selected from the entire process and should not be considered as indicative of the entire procedure. If no readings are included, the calibration consists of tolerance tests which are pass/fail. In this case, all tests are considered to be pass, unless stated otherwise.

Serial Number

VXP-02467

As received this cycle

Physical	Good
Operational	Yes
As returned	Serviced, Calibrated
Location	Laboratory
Temperature	72F
Humidity	30%

Submitted by:

DTS SPA

Rodrigo de Araya 1263

Santiago 7810161, Chile

Phone Number: 5623971072

Date Received: 01/13/2025

Order Number: PO-59134

Tested all functions in accordance with OEM Maintenance Manual.

Instrument meets all specifications and it in calibration. Unit is OK for service.

TAG ID	Standard Traceability Number	Serial Number	Model / Type	Date Calibrated	Date Due
4	124277	2580	Model 11 Calibrator	10/8/2024	10/8/2025
16	124118	52252	7310 Velocimeter	9/10/2024	9/10/2025
42	124122	48670	7310 Velocimeter	9/10/2024	9/10/2025
9	124294	1593	135M-12 Strobex	10/14/2024	10/14/2025
7	124278	2032	11800-3 Optical Tracker	10/8/2024	10/8/2025
119	149588.01	59280473MV	115 Multimeter Fluke	3/18/2024	3/18/2025

The standards used in this calibration are traceable to the National Institute Standards and Technology, appropriate industry standards where no national standard is established, or self-calibrating ratio techniques where required. This traceability is provided by documentation with Diagnostic Solutions International LLC. This certificate shall not be reproduced, except in full, without written approval from Diagnostic Solutions International LLC. Any readings or calibration date included with this certificate of calibration were recorded at the time of measurement and shall not imply anything about future accuracy. All accuracy must be determined by appropriate statistical methods. These readings are randomly selected from the entire calibration process. The collective uncertainty of each measured parameter, to include, but not solely limited to, standard accuracy, transfer uncertainty, temperature effects, procedure methods, and technician effects, of this calibration report has been determined to be at least four times lower, unless otherwise stated, than the stated accuracy, as defined by calibration procedure, of the instrument herein being calibrated.

This certificate and any included reports shall not be reproduced, except in full, without the written approval of Diagnostic Solutions.

Technician:

K.Randall

Quality Control Approval

HONEYWELL "CHADWICK" CBM HUMS / VIBREX / SKY CONNECT / ASPIRE / WORLDWIDE SALES & SUPPORT

909.930.3600 | 877.374.5521 | Fax 909.930.3323 | chadwick@dsi-hums.com | dsi-hums.com

2580 E. Philadelphia Street, Unit C, Ontario, California 91761 United States

ISO9001, AS9100 Certified Company

48067, Rev D



DIAGNOSTIC
SOLUTIONS
INTERNATIONAL LLC

Certificate of Calibration

Certificate: +125178
RMA# 250022
Date Calibrated 3/6/2025
Due Date 3/6/2026

Manufacturer

Honeywell / Chadwick Helmuth

Model

VXP Display Unit

Calibration Interval

12 months

Part Number

901-17330-1

Type

Display Unit

If any readings appear below, they are randomly selected from the entire process and should not be considered as indicative of the entire procedure. If no readings are included, the calibration consists of tolerance tests which are pass/fail. In this case, all tests are considered to be pass, unless stated otherwise.

Serial Number

D1111

As received this cycle

Physical	Good
Operational	Yes
As returned	Calibrated
Location	Laboratory
Temperature	72F
Humidity	30%

Submitted by:

DTS SPA

Rodrigo de Araya 1263

Santiago 7810161, Chile

Phone Number: 5623971072

Date Received: 01/13/2025

Order Number: PO-59134

Tested all functions in accordance with OEM Maintenance Manual.

Instrument meets all specifications and it in calibration. Unit is OK for service.

TAG ID	Standard Traceability Number	Serial Number	Model / Type	Date Calibrated	Date Due
4	124277	2580	Model 11 Calibrator	10/8/2024	10/8/2025
16	124118	52252	7310 Velocimeter	9/10/2024	9/10/2025
42	124122	48670	7310 Velocimeter	9/10/2024	9/10/2025
9	124294	1593	135M-12 Strobex	10/14/2024	10/14/2025
7	124278	2032	11800-3 Optical Tracker	10/8/2024	10/8/2025
119	149588.01	59280473MV	115 Multimeter Fluke	3/18/2024	3/18/2025

The standards used in this calibration are traceable to the National Institute Standards and Technology, appropriate industry standards where no national standard is established, or self-calibrating ratio techniques where required. This traceability is provided by documentation with Diagnostic Solutions International LLC. This certificate shall not be reproduced, except in full, without written approval from Diagnostic Solutions International LLC. Any readings or calibration date included with this certificate of calibration were recorded at the time of measurement and shall not imply anything about future accuracy. All accuracy must be determined by appropriate statistical methods. These readings are randomly selected from the entire calibration process. The collective uncertainty of each measured parameter, to include, but not solely limited to, standard accuracy, transfer uncertainty, temperature effects, procedure methods, and technician effects, of this calibration report has been determined to be at least four times lower, unless otherwise stated, than the stated accuracy, as defined by calibration procedure, of the instrument herein being calibrated.

This certificate and any included reports shall not be reproduced, except in full, without the written approval of Diagnostic Solutions.

Technician:

K. Randall

Quality Control Approval

HONEYWELL "CHADWICK" CBM HUMS / VIBREX / SKY CONNECT / ASPIRE / WORLDWIDE SALES & SUPPORT

909.930.3600 | 877.374.5521 | Fax 909.930.3323 | chadwick@dsi-hums.com | dsi-hums.com

2580 E. Philadelphia Street, Unit C, Ontario, California 91761 United States

ISO9001, AS9100 Certified Company

48067, Rev D



DIAGNOSTIC
SOLUTIONS
INTERNATIONAL LLC

Certificate of Calibration

Certificate: +125179
RMA# 250022
Date Calibrated 3/6/2025
Due Date 3/6/2026

Manufacturer

Honeywell / Chadwick Helmuth

Model

11800-3

Calibration Interval

12 months

Part Number

901-11800-3

Type

Fastrak

If any readings appear below, they are randomly selected from the entire process and should not be considered as indicative of the entire procedure. If no readings are included, the calibration consists of tolerance tests which are pass/fail. In this case, all tests are considered to be pass, unless stated otherwise.

Serial Number

6256

As received this cycle

Physical	Good
Operational	Yes
As returned	Calibrated
Location	Laboratory
Temperature	72F
Humidity	30%

Submitted by:

DTS SPA

Rodrigo de Araya 1263

Santiago 7810161, Chile

Phone Number: 5623971072

Date Received: 01/13/2025

Order Number: PO-59134

Tested all functions in accordance with OEM Maintenance Manual.

Instrument meets all specifications and it in calibration. Unit is OK for service.

TAG ID	Standard Traceability Number	Serial Number	Model / Type	Date Calibrated	Date Due
4	124277	2580	Model 11 Calibrator	10/8/2024	10/8/2025
16	124118	52252	7310 Velocimeter	9/10/2024	9/10/2025
42	124122	48670	7310 Velocimeter	9/10/2024	9/10/2025
63	150875.02	3922A09499	8904A Synthesizer	5/1/2024	5/1/2025
20	155298.01	2735A04283	3561A Signal Analyzer	10/29/2024	10/29/2025
119	149588.01	59280473MV	115 Multimeter Fluke	3/18/2024	3/18/2025
5	124279	1635	8500C Balancer / Analyzer	10/8/2024	10/8/2025

The standards used in this calibration are traceable to the National Institute Standards and Technology, appropriate industry standards where no national standard is established, or self-calibrating ratio techniques where required. This traceability is provided by documentation with Diagnostic Solutions International LLC. This certificate shall not be reproduced, except in full, without written approval from Diagnostic Solutions International LLC. Any readings or calibration date included with this certificate of calibration were recorded at the time of measurement and shall not imply anything about future accuracy. All accuracy must be determined by appropriate statistical methods. These readings are randomly selected from the entire calibration process. The collective uncertainty of each measured parameter, to include, but not solely limited to, standard accuracy, transfer uncertainty, temperature effects, procedure methods, and technician effects, of this calibration report has been determined to be at least four times lower, unless otherwise stated, than the stated accuracy, as defined by calibration procedure, of the instrument herein being calibrated.

This certificate and any included reports shall not be reproduced, except in full, without the written approval of Diagnostic Solutions.

Technician:

K.Randall

Quality Control Approval

HONEYWELL "CHADWICK" CBM HUMS / VIBREX / SKY CONNECT / ASPIRE / WORLDWIDE SALES & SUPPORT

909.930.3600 | 877.374.5521 | Fax 909.930.3323 | chadwick@dsi-hums.com | dsi-hums.com

2580 E. Philadelphia Street, Unit C, Ontario, California 91761 United States

ISO9001, AS9100 Certified Company

48067, Rev D



DIAGNOSTIC
SOLUTIONS
INTERNATIONAL LLC

Certificate of Calibration

Certificate: +125180
RMA# 250022
Date Calibrated 3/6/2025
Due Date 3/6/2026

Manufacturer

Honeywell / Chadwick Helmuth

Model

10200-1

Calibration Interval

12 months

Part Number

901-10200-1

Type

Probe Photocell

If any readings appear below, they are randomly selected from the entire process and should not be considered as indicative of the entire procedure. If no readings are included, the calibration consists of tolerance tests which are pass/fail. In this case, all tests are considered to be pass, unless stated otherwise.

Serial Number

8114

As received this cycle

Physical	Good
Operational	Yes
As returned	Calibrated
Location	Laboratory
Temperature	72F
Humidity	30%

Submitted by:

DTS SPA

Rodrigo de Araya 1263

Santiago 7810161, Chile

Phone Number: 5623971072

Date Received: 01/13/2025

Order Number: PO-59134

Tested all functions in accordance with OEM Maintenance Manual.

Instrument meets all specifications and it in calibration. Unit is OK for service.

TAG ID	Standard Traceability Number	Serial Number	Model / Type	Date Calibrated	Date Due
4	124277	2580	Model 11 Calibrator	10/8/2024	10/8/2025
11	124295	1241	10170-1 Processor	10/14/2024	10/14/2025
119	149588.01	59280473MV	115 Multimeter Fluke	3/18/2024	3/18/2025
5	124279	1635	8500C Balancer / Analyzer	10/8/2024	10/8/2025

The standards used in this calibration are traceable to the National Institute Standards and Technology, appropriate industry standards where no national standard is established, or self-calibrating ratio techniques where required. This traceability is provided by documentation with Diagnostic Solutions International LLC. This certificate shall not be reproduced, except in full, without written approval from Diagnostic Solutions International LLC. Any readings or calibration date included with this certificate of calibration were recorded at the time of measurement and shall not imply anything about future accuracy. All accuracy must be determined by appropriate statistical methods. These readings are randomly selected from the entire calibration process. The collective uncertainty of each measured parameter, to include, but not solely limited to, standard accuracy, transfer uncertainty, temperature effects, procedure methods, and technician effects, of this calibration report has been determined to be at least four times lower, unless otherwise stated, than the stated accuracy, as defined by calibration procedure, of the instrument herein being calibrated.

This certificate and any included reports shall not be reproduced, except in full, without the written approval of Diagnostic Solutions.

Technician:

K.Randall

Quality Control Approval

HONEYWELL "CHADWICK" CBM HUMS / VIBREX / SKY CONNECT / ASPIRE / WORLDWIDE SALES & SUPPORT

909.930.3600 | 877.374.5521 | Fax 909.930.3323 | chadwick@dsi-hums.com | dsi-hums.com

2580 E. Philadelphia Street, Unit C, Ontario, California 91761 United States

ISO9001, AS9100 Certified Company

48067, Rev D



(909) 930-3600
2580 E. Philadelphia St.
Unit C
Ontario, CA 91761

Certificate of Calibration

Certificate No. + 125181
RMA No. 250022
Date Calibrated 3/6/2025
Due Date 3/6/2026

Sensor Information:

Model Number 7310
Serial Number 92606

Manufacturer Honeywell
Part Number 901-7310
Type Velocimeter

Calibration Data

Sensitivity @ 100 Hz: 18.06 mV/in/s
Test Level: 1.00 in/s pk
Pass/Fail: PASS


Lab Conditions

Temperature: 68 °F
Humidity: 30 %

Transducer Specifications

Amp. Range: 19.0 (± 5%) mV/IPS
Sensor Tolerance: 5 - <20 Hz(+6%, -7%) mV/IPS
20-1000 Hz (± 5%) mV/IPS
Resonant Freq: ≥ 17 KHz
Temp. Range: -40 to 125 °C

Deviation Plot

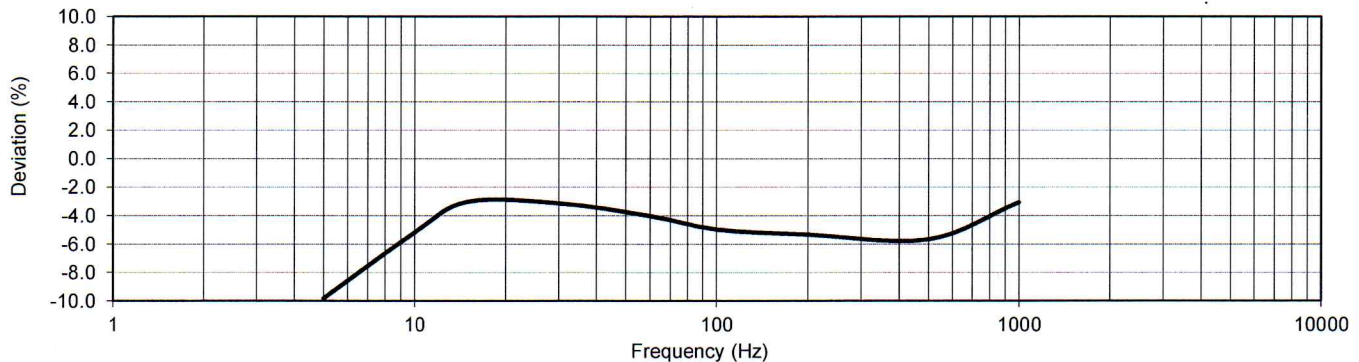

Data Table

Frequency (Hz)	Deviation (%)	Max Deviation allowed *
5	-9.82	-12% +11%
10	-5.20	-12% +11%
15	-3.02	-12% +11%
30	-3.13	8%
60	-4.01	8%
100	-4.96	8%
200	-5.33	8%
500	-5.67	8%
1000	-3.07	8%

Unit Condition

As Received: In Tolerance

As Returned: In Tolerance

Customer:

DTS SPA
Rodrigo de Araya 1263
Santiago 7810161, Chile

Phone Number:

5623971072

Date Received:

1/13/2025

Order Number:

PO-59134

User Notes

Tested all functions IAW OEM maintenance manual.
Instrument meets all specifications and is in calibration.
Unit is OK for service

Traceability

Model No. 25930
Serial Number: 100
Calibration Date: 6/13/2024
Calibration Due Date: 6/13/2025
PTB: Project 17014 and 17004
NIST: Project 683/287323

The standards used in this calibration are traceable to the National Institute of Standards and Technology, appropriate industry standards where no national standard is established, or self calibrating ratio techniques where required. This Traceability is provided by documentation with Diagnostic Solutions LLC.

Any readings or calibration date included with this certificate of calibration were recorded at the time of measurement and shall not imply anything about future accuracy. All accuracy must be determined by appropriate statistical methods. These readings are randomly selected from the entire calibration process. The collective uncertainty of each measured parameter, to include, but not solely limited to, standard accuracy, transfer uncertainty, temperature effects, procedure methods, and technician effects, of this calibration report has been determined to be at least four times lower, unless otherwise stated, than the stated accuracy, as defined by calibration procedure, of the instrument herein being calibrated.

This certificate and any included reports shall not be reproduced, except in full, without the written approval of Diagnostic Solutions.

Technician Signature

Keith Randall


Quality Control Approval

* Includes Shaker Tolerance



Certificate No. + 125182
RMA No. 250022
Date Calibrated 3/6/2025
Due Date 3/6/2026

Amp. Range:	19.0 (± 5%)	mV/IPS
Sensor Tolerance:	5 - <20 Hz(+6%, -7%)	mV/IPS
	20-1000 Hz (± 5%)	mV/IPS
Resonant Freq:	≥ 17	KHz
Temp. Range:	-40 to 125	°C

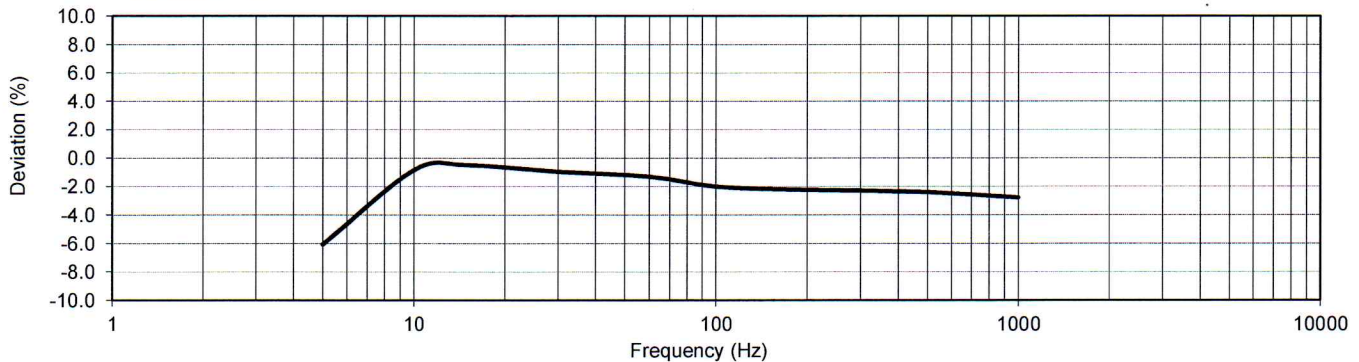

Diagnostic Solutions International, LLC | 25996, REV M (ECO-2744)



(909) 930-3600
2580 E. Philadelphia St.
Unit C
Ontario, CA 91761

Certificate of Calibration

Certificate No. + 125183

RMA No. 250022

Date Calibrated 3/6/2025

Due Date 3/6/2026

Sensor Information:

Model Number 7310
Serial Number 92607

Manufacturer Honeywell
Part Number 901-7310
Type Velocimeter

Calibration Data


Sensitivity @ 100 Hz: 17.96 mV/in/s
Test Level: 1.00 in/s pk
Pass/Fail: PASS

Lab Conditions
Temperature: 68 °F
Humidity: 30 %

Transducer Specifications

Amp. Range: 19.0 (± 5%) mV/IPS
Sensor Tolerance: 5 - <20 Hz(+6%, -7%) mV/IPS
20-1000 Hz (± 5%) mV/IPS
Resonant Freq: ≥ 17 KHz
Temp. Range: -40 to 125 °C

Deviation Plot

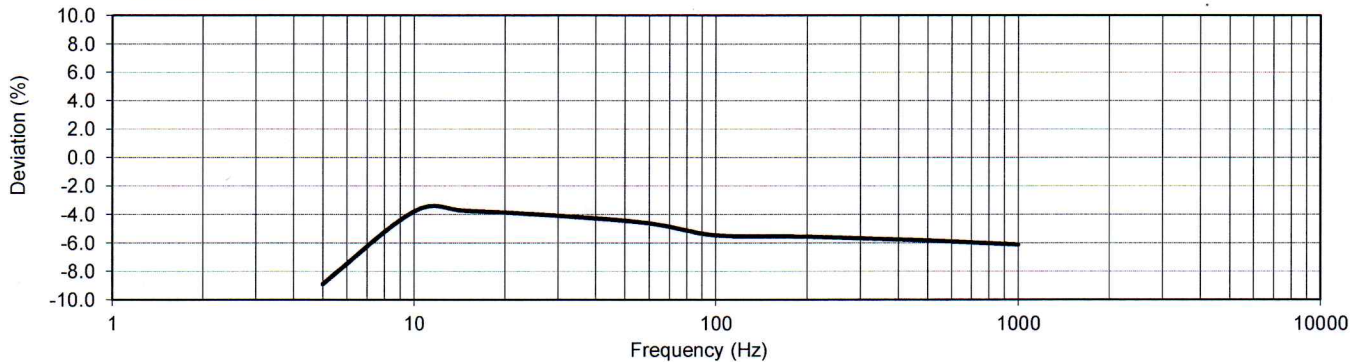

Data Table

Frequency (Hz)	Deviation (%)	Max Deviation allowed *
5	-8.89	-12% +11%
10	-3.78	-12% +11%
15	-3.74	-12% +11%
30	-4.08	8%
60	-4.61	8%
100	-5.45	8%
200	-5.56	8%
500	-5.83	8%
1000	-6.11	8%

Unit Condition

As Received: In Tolerance

As Returned: In Tolerance

Customer:

DTS SPA
Rodrigo de Araya 1263
Santiago 7810161, Chile

Phone Number:

5623971072

Date Received:

1/13/2025

Order Number:

PO-59134

User Notes

Tested all functions IAW OEM maintenance manual.
Instrument meets all specifications and is in calibration.
Unit is OK for service

Traceability

Model No. 25930
Serial Number: 100
Calibration Date: 6/13/2024
Calibration Due Date: 6/13/2025
PTB: Project 17014 and 17004
NIST: Project 683/287323

The standards used in this calibration are traceable to the National Institute of Standards and Technology, appropriate industry standards where no national standard is established, or self calibrating ratio techniques where required. This Traceability is provided by documentation with Diagnostic Solutions LLC.

Any readings or calibration date included with this certificate of calibration were recorded at the time of measurement and shall not imply anything about future accuracy. All accuracy must be determined by appropriate statistical methods. These readings are randomly selected from the entire calibration process. The collective uncertainty of each measured parameter, to include, but not solely limited to, standard accuracy, transfer uncertainty, temperature effects, procedure methods, and technician effects, of this calibration report has been determined to be at least four times lower, unless otherwise stated, than the stated accuracy, as defined by calibration procedure, of the instrument herein being calibrated.

This certificate and any included reports shall not be reproduced, except in full, without the written approval of Diagnostic Solutions.

Technician Signature

Keith Randall

Quality Control Approval

* Includes Shaker Tolerance