MICRO PRECISION CALIBRATION INC.
9080 ACTIVITY RD. STE C
SAN DIEGO CA 92126
858-547-0217

# Certificate of Calibration

**Date: Aug 10, 2026**

**Cert No. 5523631063120232**

**Customer:**

FUERZA AEREA DE CHILE

RODRIGO DE ARAYA # 1263
SANTIAGO CHILE 7810161

| | | | |
|---|---|---|---|
| | | Work Order #: | SD-50059770 |
| | | Purchase Order #: | 62472 |
| MPC Control #: | 31995 | Serial Number: | 31995 |
| Asset ID: | 31995 | Department: | N/A |
| Gage Type: | TRANSDUCER VIBRATION VELOCITY | Performed By: | MIGUEL MATA |
| Manufacturer: | CEC | Received Condition: | IN TOLERANCE |
| Model Number: | 09384/4-123-0001 | Returned Condition: | IN TOLERANCE |
| Size: | 45 to 2000 Hz | Cal. Date: | August 10, 2026 |
| Temp/RH: | 22.6°C / 62.2% | Cal. Interval: | 12 MONTHS |
| Location: | Calibration performed at MPC facility | Cal. Due Date: | August 10, 2027 |

**Calibration Notes:**

Instrument calibrated in accordance with manufacturer's specifications.
See attached calibration data (1 page).
Procedure used as reference.

## Standards Used to Calibrate Equipment

| I.D. | Description. | Model | Serial | Manufacturer | Cal. Due Date | Traceability # |
|---|---|---|---|---|---|---|
| BQ4563 | DECADE RESISTOR | 1432-A | 6261 | GENERAL RADIO | Aug 31, 2026 | 5523631032134561 |
| DE5574 | DIGITAL MULTIMETER | 3458A | 2823A14502 | HEWLETT PACKARD | Jun 30, 2027 | 5523631035915349 |
| P1630 | TRANSDUCER TEST SET | HI 803 | 0355 | HARDY INSTRUMENTS | Jun 30, 2027 | 5523631035899917 |

## Procedures Used in this Event

| Procedure Name | Description |
|---|---|
| MPC-VIB-001 Rev. 06 | Accelerometers, General, Rev.06, Jun-07-2024 |

Calibrating Technician:



MIGUEL MATA

QC Approval:



JESSE GARCIA

**STATEMENTS OF PASS OR FAIL CONFORMANCE:** The uncertainty of measurement has been taken into account when determining compliance with specification. All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in compliance with ANSI/NCSL Z540.3-2006.

**THE CALIBRATION REPORT STATUS:**
**PASS**- Term used when compliance statement is given, and the measurement result is PASS.
**PASS²**- Term used when compliance statement is given, and the measurement result is conditional passed or PASS².
**FAIL**- Term used when compliance statement is given, and the measurement result is FAIL.
**FAIL²**- Term used when compliance statement is given, and the measurement result is conditional failed or FAIL².
**REPORT OF VALUE** - Term used when reported measurement is not requiring compliance statement in report.
**ADJUSTED**- When adjustments are made to an instrument which changes the value of measurement from what was measured as found to new value as left.
**LIMITED** - When an instrument fails calibration but is still functional in a limited manner.

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%, unless otherwise stated.
This calibration report complies with ISO/IEC 17025:2017, ANSI/NCSL Z540.3-2006 and ANSI/NCSL Z540.1-1994. Calibration cycles and resulting due dates were submitted/approved by the customer. Any number of factors may cause an instrument to drift out of tolerance before the next scheduled calibration. Recalibration cycles should be based on frequency of use, environmental conditions and customer's established systematic accuracy. All standards are traceable to SI through the National Institute of Standards and Technology (NIST) and/or recognized national or international standards laboratories. Services rendered include proper manufacturer's service instruction and are warranted for no less than thirty (30) days. The information on this report pertains only to the instrument identified, this may not be reproduced in part or in a whole without the prior written approval of the issuing MP Calibration Laboratory.



(CERT, Rev 9)

MICRO PRECISION

# Calibration Report of CEC 09384/4-123-0001 Transducer Vibration Velocity

| | | | |
|---|---|---|---|
| MPC Control #: | 31995 | Serial Number: | 31995 |
| Asset ID: | 31995 | Calibration Date: | August 10, 2026 |

## Acceleration Measurement

*Reference Sensitivity / Mass 112.49 grams*

| Applied Setting | UUT Spec Sensitivity | Lower Limit | As Found | As Left | Upper Limit | Result |
|---|---|---|---|---|---|---|
| 100 Hz @ 1 in/sec | 135.0 mV | 133.0000 mV | 133.2192 mV | 133.2192 mV | 137.0000 mV | PASS |

*Frequency Response*

*Referenced to 100 Hz Output*


| Applied Setting | UUT Ref Sensitivity | Lower Limit | As Found | As Left | Upper Limit | Result |
|---|---|---|---|---|---|---|
| 45 Hz @ 1 in/sec | 133.2192 mV | 122.5617 mV | 132.9813 mV | 132.9813 mV | 143.8767 mV | PASS |
| 1000 Hz @ 1 in/sec | 133.2192 mV | 122.5617 mV | 133.1534 mV | 133.1534 mV | 143.8767 mV | PASS |
| 1500 Hz @ 1 in/sec | 133.2192 mV | 122.5617 mV | 134.1637 mV | 134.1637 mV | 143.8767 mV | PASS |
| 2000 Hz @ 1 in/sec | 133.2192 mV | 122.5617 mV | 134.7280 mV | 134.7280 mV | 143.8767 mV | PASS |

## Statements of Pass or Fail Conformance

**The status of compliance with the acceptance criteria is reported as:**

**PASS** — Compliant with specification.

**FAIL** — Not compliant with specification.

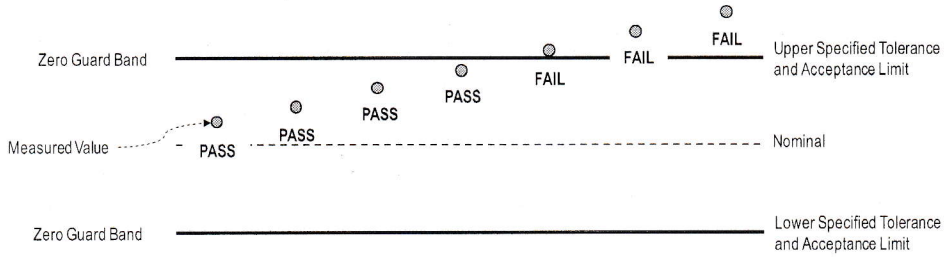


**Acceptance limits equal to the tolerance limits**

**- End of Calibration Report -**

**Confidential:** Controlled Document.
Cannot be reproduced without the approval of the Quality Department.