MICRO PRECISION CALIBRATION INC.
9080 ACTIVITY RD. STE C
SAN DIEGO CA 92126
858-547-0217

Certificate of Calibration

Date: Aug 10, 2026 **Cert No. 5523631063120186**

Customer:

FUERZA AEREA DE CHILE
RODRIGO DE ARAYA # 1263
SANTIAGO CHILE 7810161

		Work Order #:	SD-50059770
		Purchase Order #:	62472
MPC Control #:	31905	Serial Number:	31905
Asset ID:	31905	Department:	N/A
Gage Type:	TRANSDUCER VIBRATION VELOCITY	Performed By:	MIGUEL MATA
Manufacturer:	CEC	Received Condition:	IN TOLERANCE
Model Number:	09384/4-123-0001	Returned Condition:	IN TOLERANCE
Size:	45 to 2000 Hz	Cal. Date:	August 10, 2026
Temp/RH:	22.6°C / 62.2%	Cal. Interval:	12 MONTHS
Location:	Calibration performed at MPC facility	Cal. Due Date:	August 10, 2027

Calibration Notes:

Instrument calibrated in accordance with manufacturer's specifications.
See attached calibration data (1 page).
Procedure used as reference.

Standards Used to Calibrate Equipment

I.D.	Description.	Model	Serial	Manufacturer	Cal. Due Date	Traceability #
BQ4563	DECADE RESISTOR	1432-A	6261	GENERAL RADIO	Aug 31, 2026	5523631032134561
DE5574	DIGITAL MULTIMETER	3458A	2823A14502	HEWLETT PACKARD	Jun 30, 2027	5523631035915349
P1630	TRANSDUCER TEST SET	HI 803	0355	HARDY INSTRUMENTS	Jun 30, 2027	5523631035899917

Procedures Used in this Event

Procedure Name	Description
MPC-VIB-001 Rev. 06	Accelerometers, General, Rev.06, Jun-07-2024

Calibrating Technician: MIGUEL MATA

QC Approval: JESSE GARCIA

STATEMENTS OF PASS OR FAIL CONFORMANCE: The uncertainty of measurement has been taken into account when determining compliance with specification. All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in compliance with ANSI/NCSL Z540.3-2006.

THE CALIBRATION REPORT STATUS:
PASS- Term used when compliance statement is given, and the measurement result is PASS.
PASS²- Term used when compliance statement is given, and the measurement result is conditional passed or PASS².
FAIL- Term used when compliance statement is given, and the measurement result is FAIL.
FAIL²- Term used when compliance statement is given, and the measurement result is conditional failed or FAIL².
REPORT OF VALUE - Term used when reported measurement is not requiring compliance statement in report.
ADJUSTED- When adjustments are made to an instrument which changes the value of measurement from what was measured as found to new value as left.
LIMITED - When an instrument fails calibration but is still functional in a limited manner.

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%, unless otherwise stated.
This calibration report complies with ISO/IEC 17025:2017, ANSI/NCSL Z540.3-2006 and ANSI/NCSL Z540.1-1994. Calibration cycles and resulting due dates were submitted/approved by the customer. Any number of factors may cause an instrument to drift out of tolerance before the next scheduled calibration. Recalibration cycles should be based on frequency of use, environmental conditions and customer's established systematic accuracy. All standards are traceable to SI through the National Institute of Standards and Technology (NIST) and/or recognized national or international standards laboratories. Services rendered include proper manufacturer's service instruction and are warranted for no less than thirty (30) days. The information on this report pertains only to the instrument identified, this may not be reproduced in part or in a whole without the prior written approval of the issuing MP Calibration Laboratory.

(CERT, Rev 9)

MICRO PRECISION

Calibration Report of CEC 09384/4-123-0001 Transducer Vibration Velocity

MPC Control #:	31905	Serial Number:	31905
Asset ID:	31905	Calibration Date:	August 10, 2026

Acceleration Measurement

Reference Sensitivity / Mass 112.30 grams

Applied Setting	UUT Spec Sensitivity	Lower Limit	As Found	As Left	Upper Limit	Result
100 Hz @ 1 in/sec	135.0 mV	133.0000 mV	135.3380 mV	135.3380 mV	137.0000 mV	PASS

Frequency Response

Referenced to 100 Hz Output


Applied Setting	UUT Ref Sensitivity	Lower Limit	As Found	As Left	Upper Limit	Result
45 Hz @ 1 in/sec	135.3380 mV	124.5109 mV	133.2971 mV	133.2971 mV	146.1650 mV	PASS
1000 Hz @ 1 in/sec	135.3380 mV	124.5109 mV	136.0955 mV	136.0955 mV	146.1650 mV	PASS
1500 Hz @ 1 in/sec	135.3380 mV	124.5109 mV	136.4349 mV	136.4349 mV	146.1650 mV	PASS
2000 Hz @ 1 in/sec	135.3380 mV	124.5109 mV	136.7376 mV	136.7376 mV	146.1650 mV	PASS

Statements of Pass or Fail Conformance

The status of compliance with the acceptance criteria is reported as:

PASS — Compliant with specification.

FAIL — Not compliant with specification.

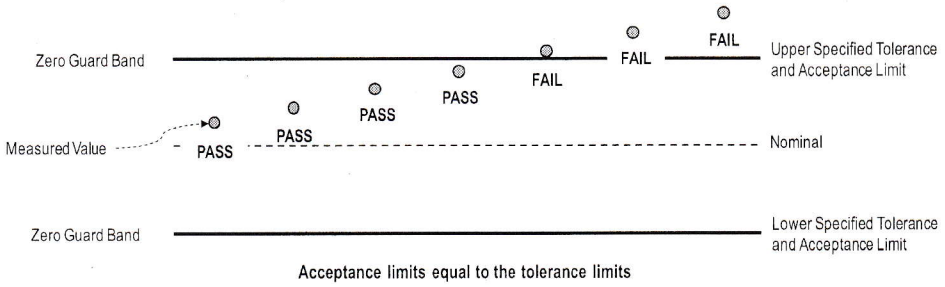

Acceptance limits equal to the tolerance limits

- End of Calibration Report -

Confidential: Controlled Document.
Cannot be reproduced without the approval of the Quality Department.