



MICRO PRECISION CALIBRATION INC.  
9080 ACTIVITY RD. STE C  
SAN DIEGO CA 92126  
858-547-0217

## Certificate of Calibration

Date: Jan 22, 2026

Cert No. 5523631032505672

### Customer:

FUERZA AEREA DE CHILE  
RODRIGO DE ARAYA # 1263  
SANTIAGO CHILE 7810161

MPC Control #: 30330  
Asset ID: 30330  
Gage Type: VIBRATION TRANSDUCER  
Manufacturer: CEC  
Model Number: 4-128-0127  
Size: 45 to 1500 Hz  
Temp/RH: 23.1°C / 45.8%  
Location: Calibration performed at MPC facility

Work Order #: SD-50056925  
Purchase Order #: PO-61134  
Serial Number: 30330  
Department: N/A  
Performed By: MIGUEL MATA  
Received Condition: IN TOLERANCE  
Returned Condition: IN TOLERANCE  
Cal. Date: January 22, 2026  
Cal. Interval: 12 MONTHS  
Cal. Due Date: January 22, 2027

### Calibration Notes:

Instrument calibrated in accordance with manufacturer's specifications.  
See attached calibration data (1 page).  
Procedure used as reference.

### Standards Used to Calibrate Equipment

| I.D.   | Description.        | Model  | Serial     | Manufacturer          | Cal. Due Date | Traceability #   |
|--------|---------------------|--------|------------|-----------------------|---------------|------------------|
| BQ4564 | DECADE RESISTOR     | 1432-L | 31612      | GENERAL RADIO COMPANY | Jul 31, 2026  | 5523631032004289 |
| DE5574 | DIGITAL MULTIMETER  | 3458A  | 2823A14502 | HEWLETT PACKARD       | Jun 30, 2026  | 5523631031930901 |
| P1630  | TRANSDUCER TEST SET | HI 803 | 0355       | HARDY INSTRUMENTS     | Jun 30, 2026  | 5523631032064641 |

### Procedures Used in this Event

Procedure Name  
MPC-VIB-001 Rev. 06

Description  
Accelerometers, General, Rev.06, Jun-07-2024

Calibrating Technician:

MIGUEL MATA

QC Approval:

JESSE GARCIA

**STATEMENTS OF PASS OR FAIL CONFORMANCE:** The uncertainty of measurement has been taken into account when determining compliance with specification. All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in compliance with ANSI/NCSL Z540.3-2006.

#### THE CALIBRATION REPORT STATUS:

**PASS:** Term used when compliance statement is given, and the measurement result is PASS.

**PASS<sup>2</sup>:** Term used when compliance statement is given, and the measurement result is conditional passed or PASS<sup>2</sup>.

**FAIL:** Term used when compliance statement is given, and the measurement result is FAIL.

**FAIL<sup>2</sup>:** Term used when compliance statement is given, and the measurement result is conditional failed or FAIL<sup>2</sup>.

**REPORT OF VALUE:** Term used when reported measurement is not requiring compliance statement in report.

**ADJUSTED:** When adjustments are made to an instrument which changes the value of measurement from what was measured as found to new value as left.

**LIMITED:** When an instrument fails calibration but is still functional in a limited manner.

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%, unless otherwise stated.  
This calibration report complies with ISO/IEC 17025:2017, ANSI/NCSL Z540.3-2006 and ANSI/NCSL Z540.1-1994. Calibration cycles and resulting due dates were submitted/approved by the customer. Any number of factors may cause an instrument to drift out of tolerance before the next scheduled calibration. Recalibration cycles should be based on frequency of use, environmental conditions and customer's established systematic accuracy. All standards are traceable to SI through the National Institute of Standards and Technology (NIST) and/or recognized national or international standards laboratories. Services rendered include proper manufacturer's service instruction and are warranted for no less than thirty (30) days. The information on this report pertains only to the instrument identified; this may not be reproduced in part or in a whole without the prior written approval of the issuing MP Calibration Laboratory.



## Calibration Report of CEC 4-128-0127 Vibration Transducer

|                |       |                   |                  |
|----------------|-------|-------------------|------------------|
| MPC Control #: | 30330 | Serial Number:    | 30330            |
| Asset ID:      | 30330 | Calibration Date: | January 22, 2026 |

### Acceleration Measurement

Reference Sensitivity / Mass 109.21 grams

| Applied Setting   | UUT Spec Sensitivity | Lower Limit | As Found    | As Left     | Upper Limit | Result |
|-------------------|----------------------|-------------|-------------|-------------|-------------|--------|
| 100 Hz @ 1 in/sec | 135.0 mV             | 126.9000 mV | 135.1769 mV | 135.1769 mV | 143.1000 mV | PASS   |

### Frequency Response


Referenced to 100 Hz Output

| Applied Setting       | UUT Ref Sensitivity | Lower Limit | As Found    | As Left     | Upper Limit | Result |
|-----------------------|---------------------|-------------|-------------|-------------|-------------|--------|
| 45 Hz @ 1 in/sec      | 135.1769 mV         | 127.0663 mV | 140.4665 mV | 140.4665 mV | 143.2875 mV | PASS   |
| 500 Hz @ 0.10 in/sec  | 135.1769 mV         | 127.0663 mV | 139.3652 mV | 139.3652 mV | 143.2875 mV | PASS   |
| 1000 Hz @ 0.10 in/sec | 135.1769 mV         | 127.0663 mV | 143.1807 mV | 143.1807 mV | 143.2875 mV | PASS   |
| 1500 Hz @ 0.10 in/sec | 135.1769 mV         | 127.0663 mV | 139.4076 mV | 139.4076 mV | 143.2875 mV | PASS   |

### Statements of Pass or Fail Conformance

The status of compliance with the acceptance criteria is reported as:

- PASS — Compliant with specification.  
FAIL — Not compliant with specification.

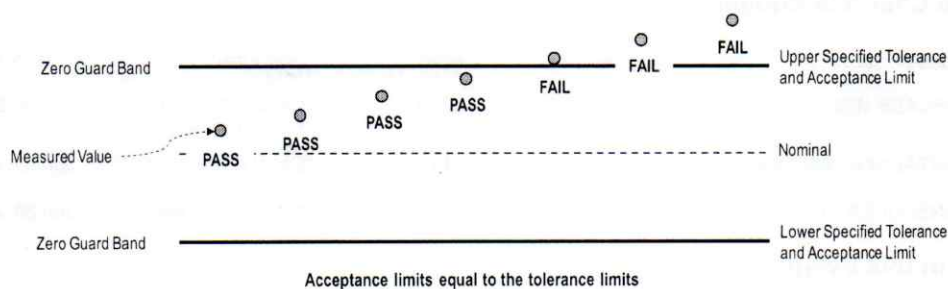

- End of Calibration Report -