



MICRO PRECISION CALIBRATION INC.
9080 ACTIVITY RD. STE C
SAN DIEGO CA 92126
858-547-0217

Certificate of Calibration

Date: Jan 22, 2026

Cert No. 5523631032505698

Customer:

FUERZA AEREA DE CHILE
RODRIGO DE ARAYA # 1263
SANTIAGO CHILE 7810161

MPC Control #: 70145
Asset ID: 70145
Gage Type: VIBRATION TRANSDUCER
Manufacturer: CEC
Model Number: 4-128-0127
Size: 45 to 1500 Hz
Temp/RH: 23.1°C / 45.8%
Location: Calibration performed at MPC facility

Work Order #: SD-50056925
Purchase Order #: PO-61134
Serial Number: 70145
Department: N/A
Performed By: MIGUEL MATA
Received Condition: IN TOLERANCE
Returned Condition: IN TOLERANCE
Cal. Date: January 22, 2026
Cal. Interval: 12 MONTHS
Cal. Due Date: January 22, 2027

Calibration Notes:

Instrument calibrated in accordance with manufacturer's specifications.
See attached calibration data (1 page).
Procedure used as reference.

Standards Used to Calibrate Equipment

I.D.	Description.	Model	Serial	Manufacturer	Cal. Due Date	Traceability #
BQ4564	DECADE RESISTOR	1432-L	31612	GENERAL RADIO COMPANY	Jul 31, 2026	5523631032004289
DE5574	DIGITAL MULTIMETER	3458A	2823A14502	HEWLETT PACKARD	Jun 30, 2026	5523631031930901
P1630	TRANSDUCER TEST SET	HI 803	0355	HARDY INSTRUMENTS	Jun 30, 2026	5523631032064641

Procedures Used in this Event

Procedure Name
MPC-VIB-001 Rev. 06

Description
Accelerometers, General, Rev.06, Jun-07-2024

Calibrating Technician:

MIGUEL MATA

QC Approval:

JESSE GARCIA

STATEMENTS OF PASS OR FAIL CONFORMANCE: The uncertainty of measurement has been taken into account when determining compliance with specification. All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in compliance with ANSI/NCSL Z540.3-2006.

THE CALIBRATION REPORT STATUS:

PASS - Term used when compliance statement is given, and the measurement result is PASS.

PASS² - Term used when compliance statement is given, and the measurement result is conditional passed or PASS².

FAIL - Term used when compliance statement is given, and the measurement result is FAIL.

FAIL² - Term used when compliance statement is given, and the measurement result is conditional failed or FAIL².

REPORT OF VALUE - Term used when reported measurement is not requiring compliance statement in report.

ADJUSTED - When adjustments are made to an instrument which changes the value of measurement from what was measured as found to new value as left.

LIMITED - When an instrument fails calibration but is still functional in a limited manner.

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%, unless otherwise stated.

This calibration report complies with ISO/IEC 17025:2017, ANSI/NCSL Z540.3-2006 and ANSI/NCSL Z540.1-1994. Calibration cycles and resulting due dates were submitted/approved by the customer. Any number of factors may cause an instrument to drift out of tolerance before the next scheduled calibration. Recalibration cycles should be based on frequency of use, environmental conditions and customer's established systematic accuracy. All standards are traceable to SI through the National Institute of Standards and Technology (NIST) and/or recognized national or international standards laboratories. Services rendered include proper manufacturer's service instruction and are warranted for no less than thirty (30) days. The information on this report pertains only to the instrument identified; this may not be reproduced in part or in a whole without the prior written approval of the issuing MP Calibration Laboratory.



Calibration Report of CEC 4-128-0127 Vibration Transducer

MPC Control #: <u>70145</u>	Serial Number: <u>70145</u>
Asset ID: <u>70145</u>	Calibration Date: <u>January 22, 2026</u>

Acceleration Measurement

Reference Sensitivity / Mass 108.65 grams

Applied Setting	UUT Spec Sensitivity	Lower Limit	As Found	As Left	Upper Limit	Result
100 Hz @ 1 in/sec	135.0 mV	126.9000 mV	134.1676 mV	134.1676 mV	143.1000 mV	PASS

Frequency Response


Referenced to 100 Hz Output

Applied Setting	UUT Ref Sensitivity	Lower Limit	As Found	As Left	Upper Limit	Result
45 Hz @ 1 in/sec	134.1676 mV	126.1175 mV	140.8010 mV	140.8010 mV	142.2176 mV	PASS
500 Hz @ 0.10 in/sec	134.1676 mV	126.1175 mV	129.1135 mV	129.1135 mV	142.2176 mV	PASS
1000 Hz @ 0.10 in/sec	134.1676 mV	126.1175 mV	135.8367 mV	135.8367 mV	142.2176 mV	PASS
1500 Hz @ 0.10 in/sec	134.1676 mV	126.1175 mV	127.1968 mV	127.1968 mV	142.2176 mV	PASS

Statements of Pass or Fail Conformance

The status of compliance with the acceptance criteria is reported as:

- PASS** — Compliant with specification.
FAIL — Not compliant with specification.

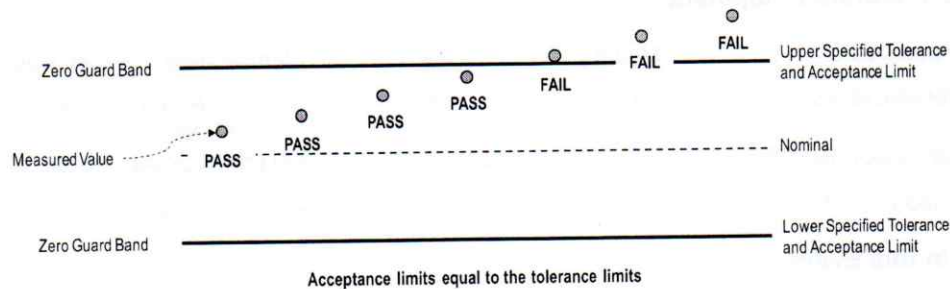

- End of Calibration Report -