



2102-08-091

8 CONTACT sEEG DEPTH

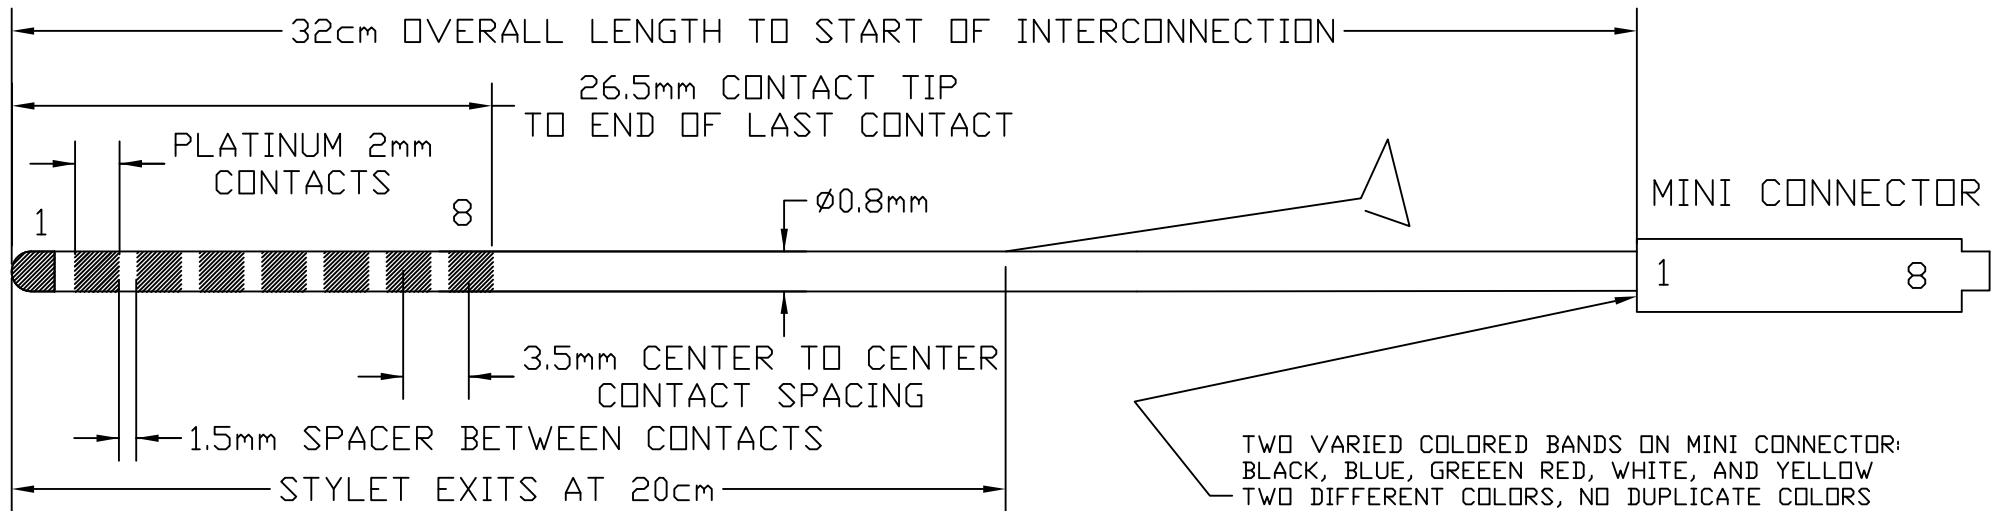

PACKAGING VIEW

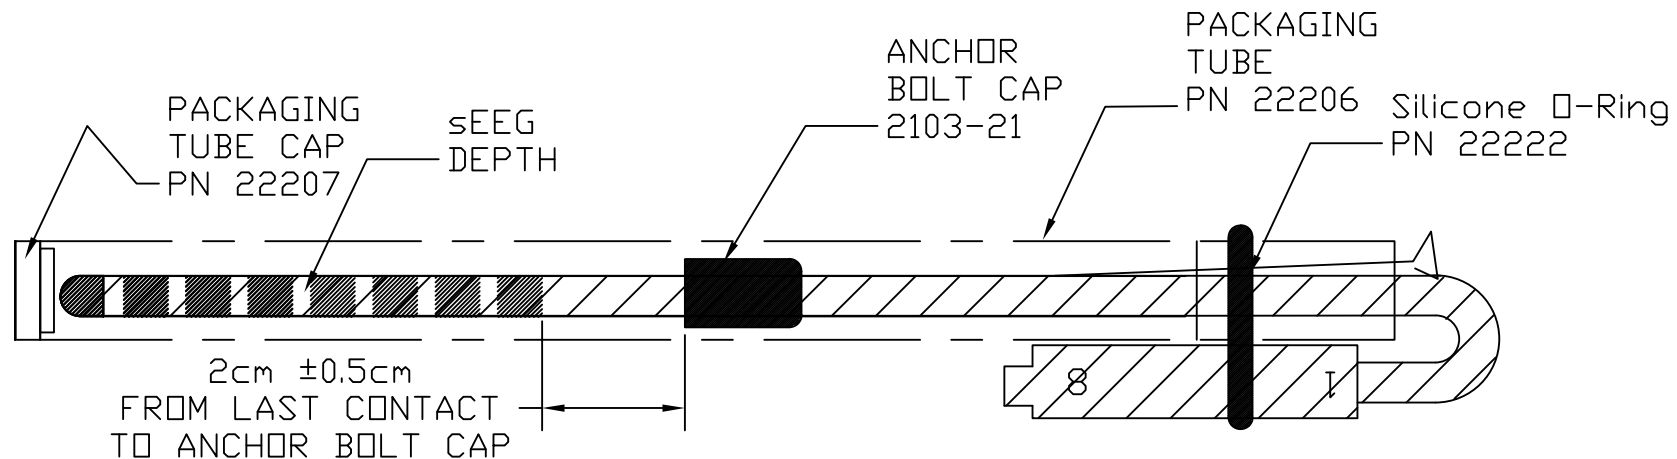

Electrode specifications may be changed without prior notice. Please always use the code charts supplied with each electrode shipment to ensure having the latest specifications

CAUTION: Federal Law (USA) restricts to the sale by or on the order of a physician

Note: It is important to place and secure a strain relief using the EEG Cable so there will not be a direct pull or stress on the electrode.

PMT Corporation

1500 PARK ROAD
CHANASSEN, MN 55317
1-800-MAN-KIND