



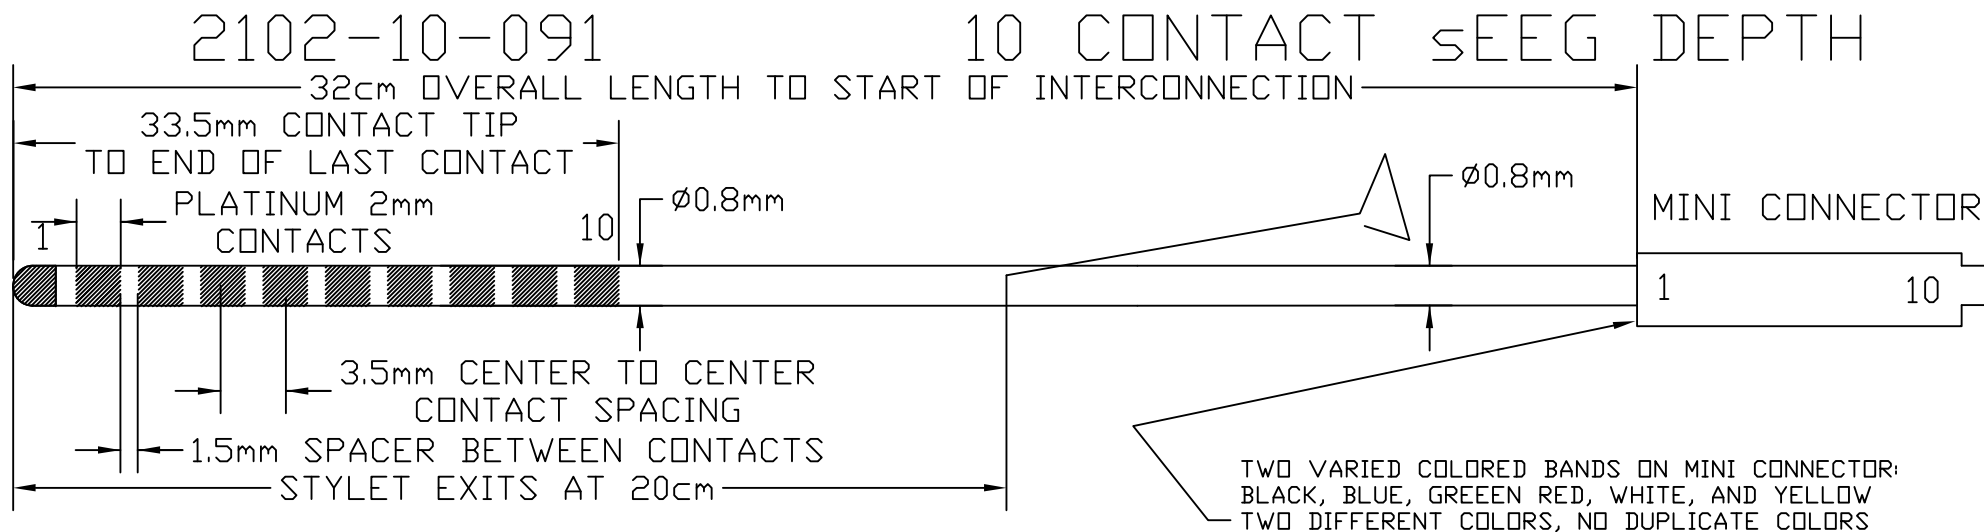

PACKAGING VIEW

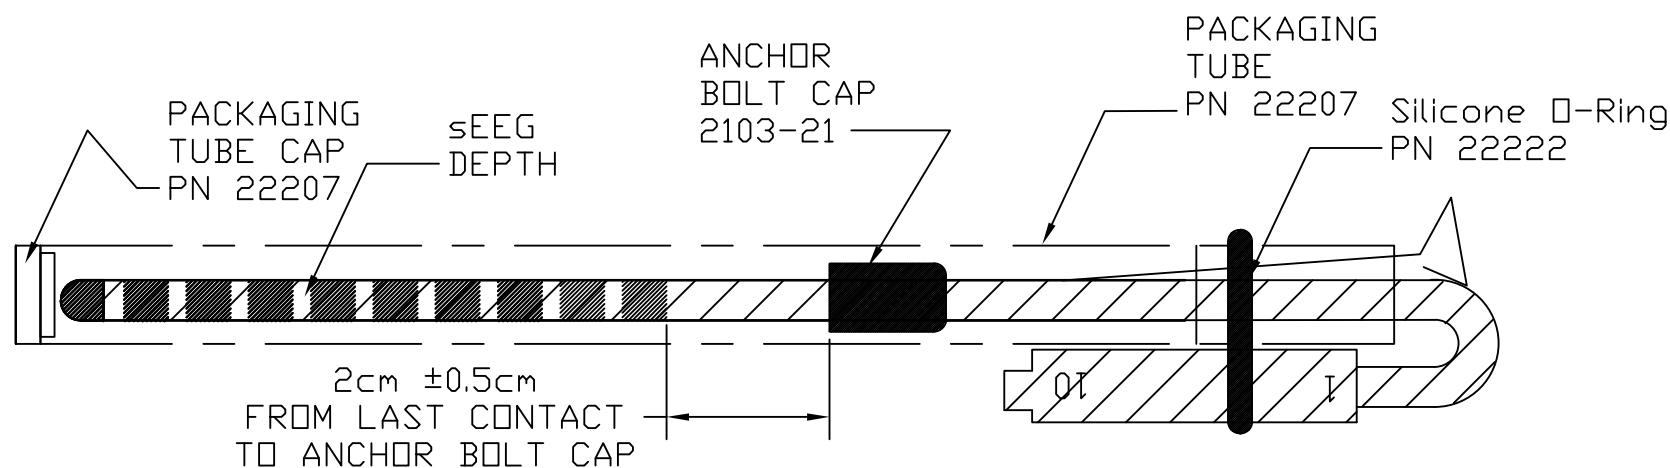

Electrode specifications may be changed without prior notice. Please always use the code charts supplied with each electrode shipment to ensure having the latest specifications

CAUTION: Federal Law (USA) restricts to the sale by or on the order of a physician

Note: It is important to place and secure a strain relief using the EEG Cable so there will not be a direct pull or stress on the electrode.