


Unique Medical

C1-60-12-05-2-A

Measures in mm

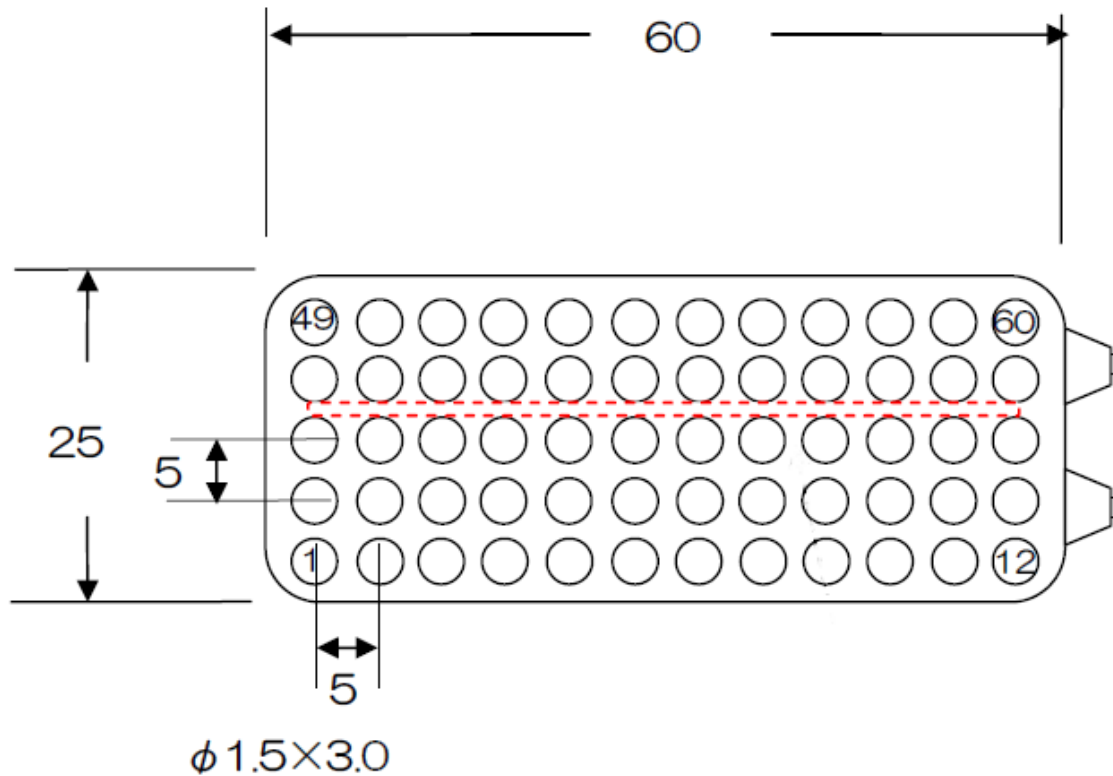

Regulation of electrode size

Subdural electrode

Inter-electrode pitch:

5 to 15 mm

External size of base:

Proportional to inter-electrode pitch

Thickness of base:


0.8 mm $\pm$ 0.2 mm

Length of lead tube:

350 mm $\pm$ 100 mm

Our intracranial electrodes can set freely number of poles, inter-poles, array, and external size.

- As we employ platinum for the electrode material it allows safe and stable measurement.
- Thickness of electrode sheet of material is 0.8 mm silicon and allows stable application.
- Electrodes can measure simultaneously 2 to 64 channels are available.

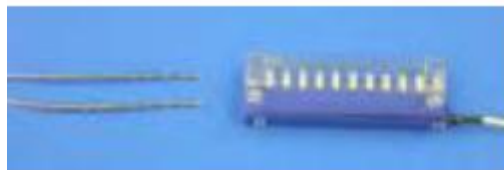

A type terminal connecting figure