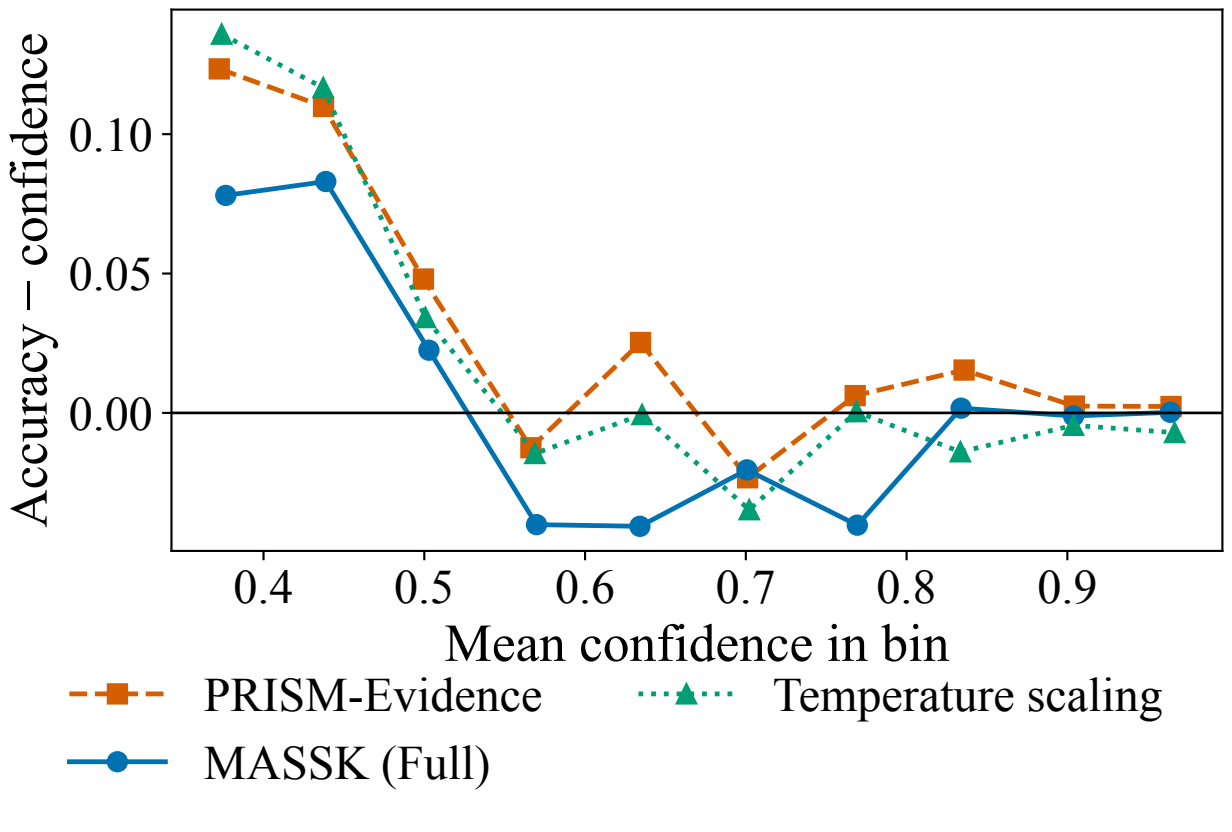
Accuracy − confidence
0.10
0.05
0.00
0.4
0.5
0.6
0.7
0.8
0.9
Mean confidence in bin
PRISM-Evidence
Temperature scaling
MASSK (Full)