



OPERATIONAL MANUAL

LAF CONTROLLER
MODEL NO: LAF153
VERSION: 1.0


NEURAL INDUSTRIAL AUTOMATION PVT LTD.,
PLOT NO: 16 Survey No: 60, Shanthi Nagar,
Near Aparna Palm Meadows,
Kompally, Hyderabad – 500 100
Telangana, INDIA

Ph: +91 79958 65752
www.neuralindustrialautomation.com


Email: [sales@ neuralindustrialautomation.in](mailto:sales@neuralindustrialautomation.in)

Dear Customer,

Thank you for choosing a NEURAL instrument, please read this operating manual carefully before you start using the instrument. This manual will provide you with all the necessary information for the correct use of the instrument as well as a precise idea of its versatility in a wide range of applications.

**Warning:**

Warnings must be followed carefully to avoid serious bodily injury.

**CAUTION:**

Cautions must be observed to avoid minor injury to yourself or damage to your equipment.

CAUTION

One three way connector is provided for power connection i.e. Line, Neutral & Earth. (100-240V AC 50/60Hz.)



Do not Switch ON power to the instrument before plugging connectors in to the terminals.



Carefully connect the connectors in the specified terminals if not it may cause damage for the instrument.

Instrument SI. No :

STANDARD PACK

1) Instruction Manual	---	1 No	☐
2) LAF153 Instrument	---	1 No	☐

Checked By :

Date :

1. Description:

LAF ON/OFF Controller is used for ON/OFF controlling of Blower, UV Lamp & CF Lamp in Dynamic pass boxes, Bio safety cabinets and laminar air flow. The status of Blower, UV Lamp & CF Lamp is provided on display.

2. Features:

- Advanced Micro controller based.
- ON/OFF Message Display
- Relay O/P for Blower (up to 1 HP), UV Lamp & CF Lamp
- ON/OFF Message status indication with high intensity Bar LEDs
- Status indication: ON, OFF-Blower, ON, OFF- UV Lamp & ON, OFF – CF Lamp
- Soft touch tactile key pad.
- Easy for Installation

3. Specifications:

GENERAL

➤ Blower Relay O/P	:	230V AC / 2 A (up to 1HP Blower can be connected).
➤ UV Lamp Relay O/P	:	230V AC / 2 A.
➤ CF Lamp Relay O/P	:	230V AC / 2 A.

RELAYS:

➤ Contact material	:	Silver Alloy.
➤ Contact Rating	:	230V AC / 2 A.
➤ No. of Operations	:	Mechanical: 10^7 , Electrical: 10^5 .

ENCLOSURE:

- Enclosure type : Power coating Box
- Mounting : Wall

LAF Controller**Display Module**

- Enclosure type : SS Northwest 4 window
- Mounting : Panel

POWER SUPPLY:

- Power : 100 - 260V, AC 50 Hz
- Wattage : 20W

ENVIRONMENTAL:

- Operating Temperature : 0 to 50°C.

4. Status Indication on Display Panel :**BLOWER:**

ON = Indicate that Blower is ON.

OFF = Indicate that Blower is OFF

BL1 FAIL= Indicate that Blower1 is failed.

BL2 FAIL= Indicate that Blower2 is failed.

BL3 FAIL= Indicate that Blower3 is failed.

BL4 FAIL= Indicate that Blower4 is failed.

**UV LAMP:**

ON = Indicate that UV LAMP is ON.

OFF = Indicate that UV LAMP is OFF

FLOURSCENT LAMP:

ON = Indicate that FLOURSCENT LAMP is ON.

OFF = Indicate that FLOURSCENT LAMP is OFF

5. Operating mode:**BLOWER:**

Press Blower push button for ON/OFF Controlling the Blower.

UV LAMP:

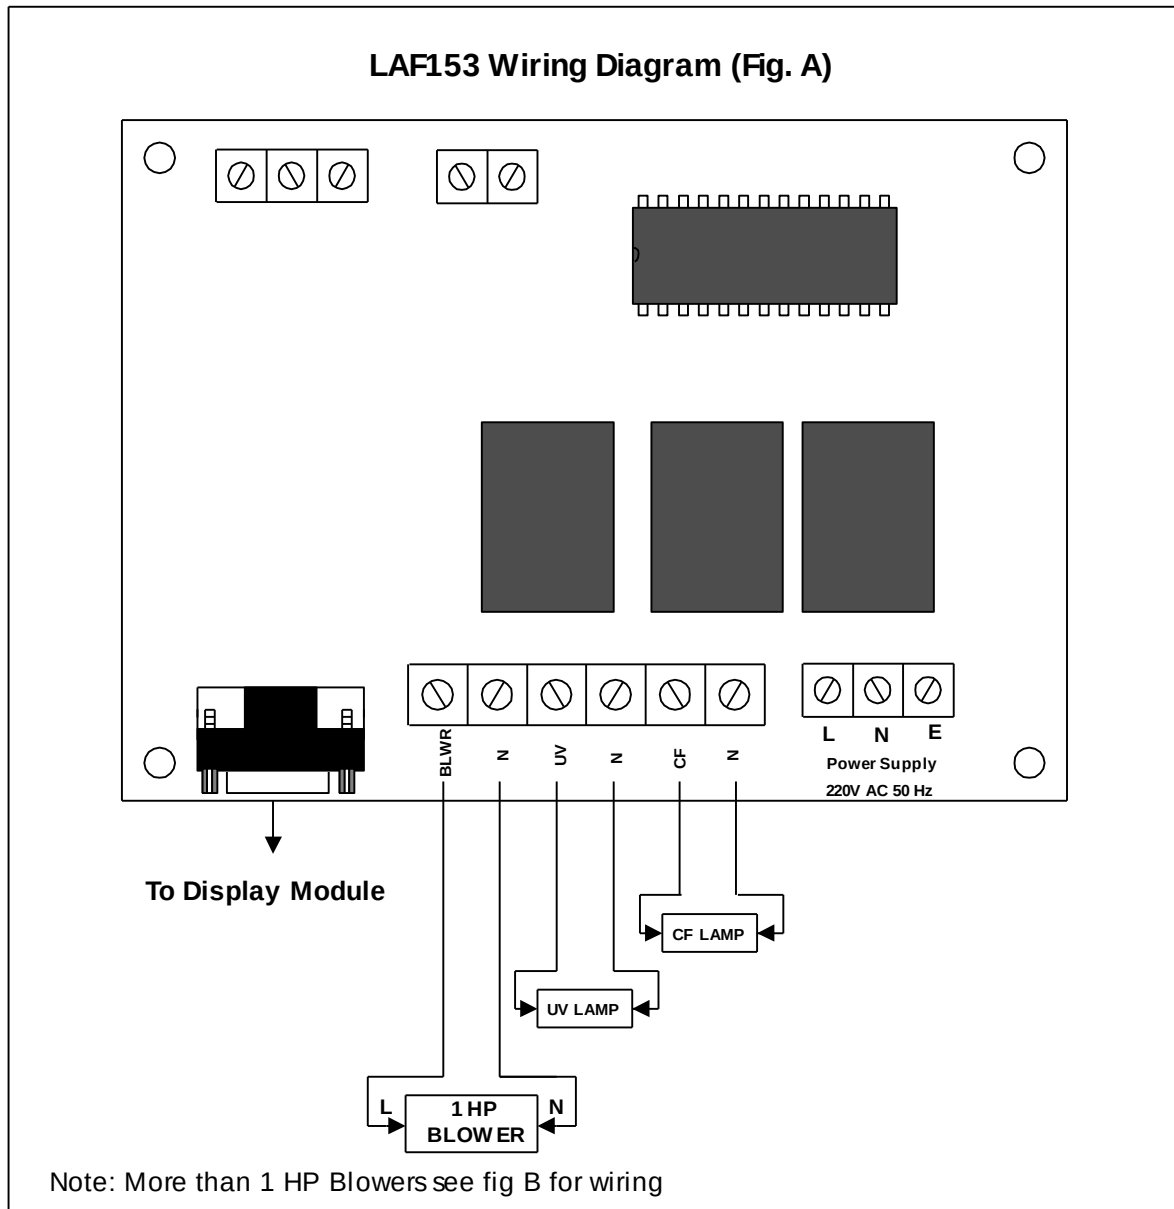
Press UV LAMP push button for ON/OFF Controlling the UV LAMP.

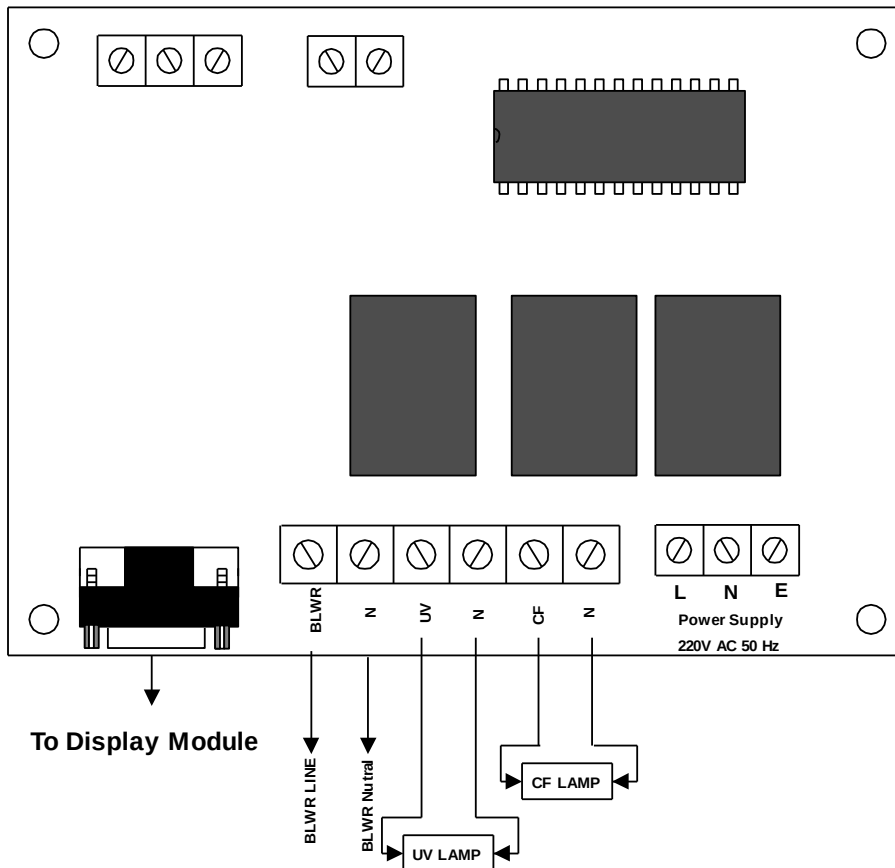
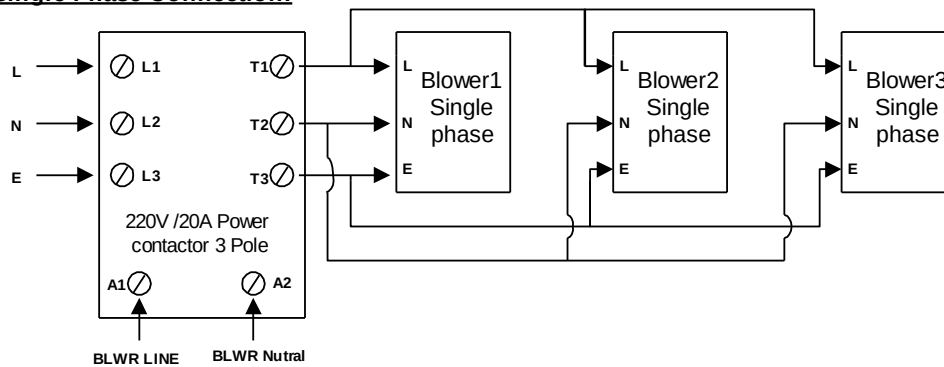
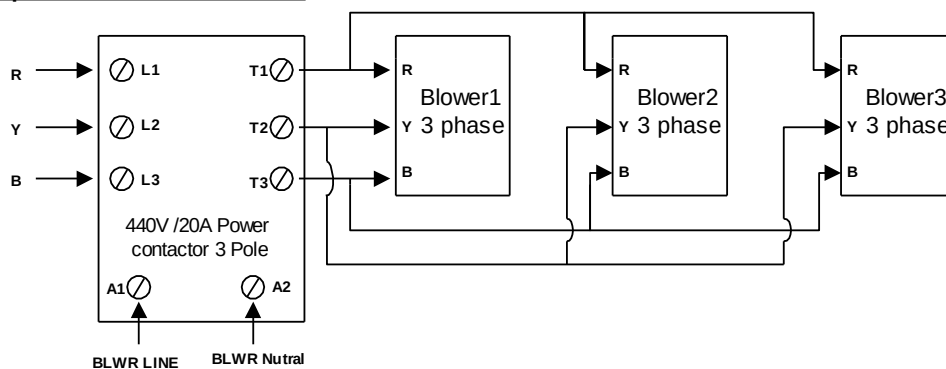
CF LAMP:

Press CF LAMP push button for ON/OFF Controlling the CF LAMP.

6. Wiring diagram:

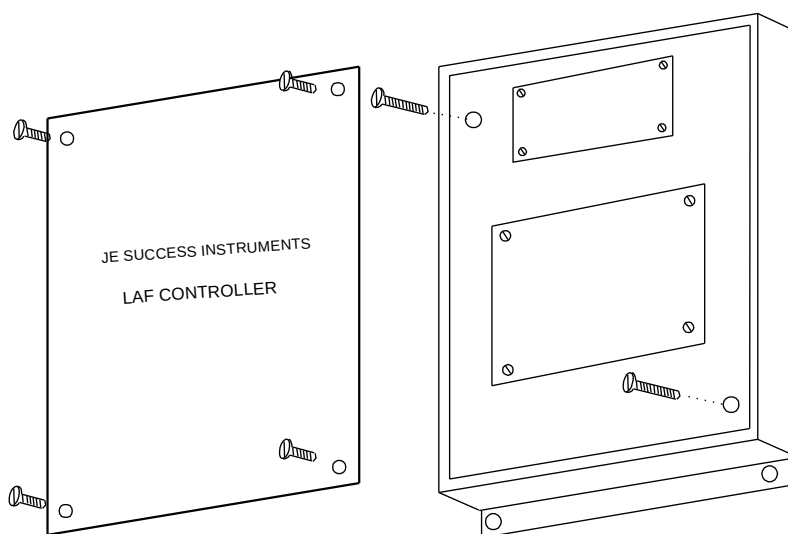
a. Wiring diagram for 1 HP Blower, UV lamp and CF lamp connection:



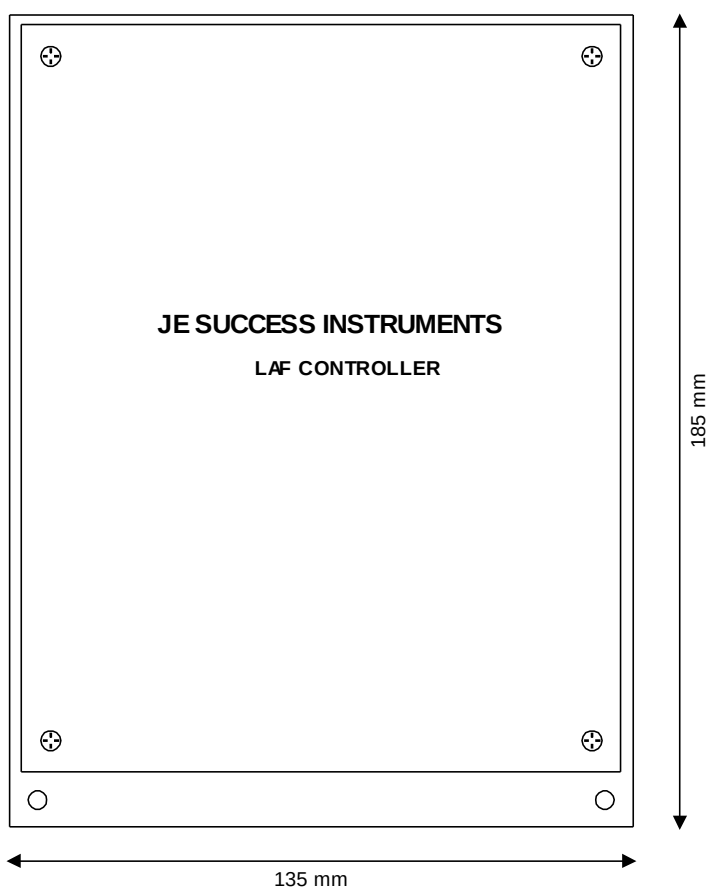
b. Wiring diagram for more than 1 HP Blowers:
LAF153 Wiring Diagram (Fig. B)
Blower Ratings more 1 HP single phase or 3 phase

Blower Single Phase Connection:

Blower3 phase Phase Connection:


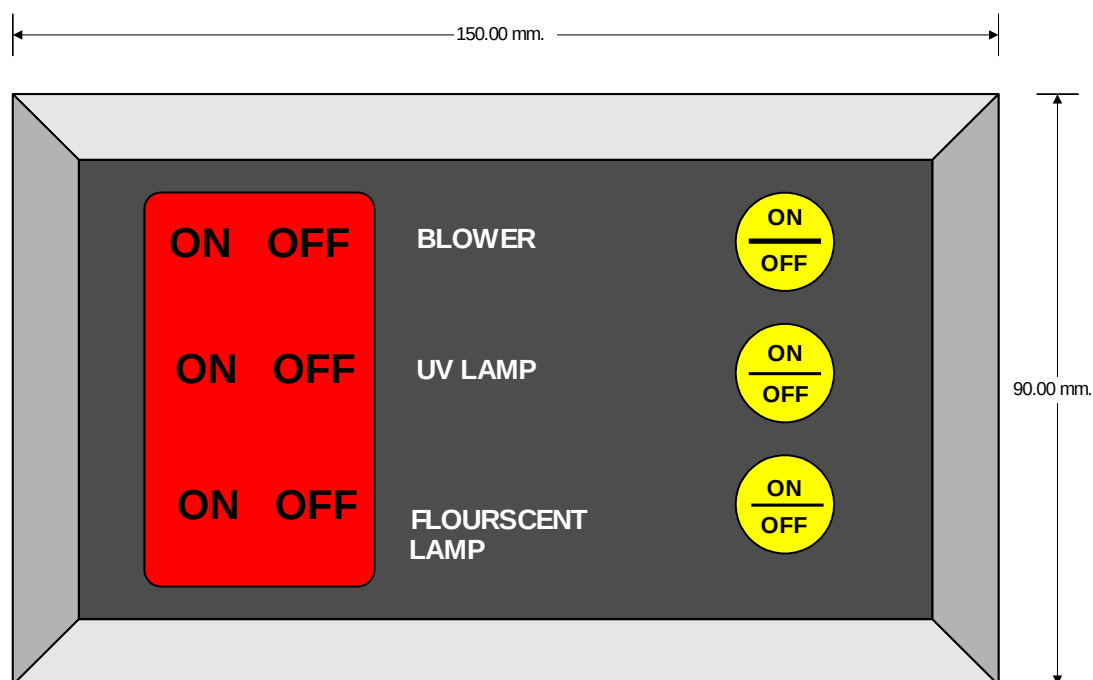
7. MECHANICAL DRAWINGS:

Figure for Installation of LAF153 Controller:



Front View Diagram of LAF153 Controller:



Front View Diagram of LAF153D:**9. Ordering Information:****I) LAF153 Controller:**

<i>Model No</i>	<i>Future use</i>
LAF153	X

Includes,

a. Controller:

<i>Model No</i>	<i>Future use</i>
LAF153	X

b. LAF153 Display Module:

<i>Model No</i>	<i>Future Use</i>
LAF153D	X

Note:

For Further Information Contact:

NEURAL INDUSTRIAL AUTOMATION PVT LTD.

PLOT NO: 16 Survey No: 60, Near Aparna Palm Meadows, Kompally, Hyderabad –500 100
Telangana, INDIA

www.neuralindustrialautomation.com

Email: [sales@ neuralindustrialautomation.in](mailto:sales@neuralindustrialautomation.in)