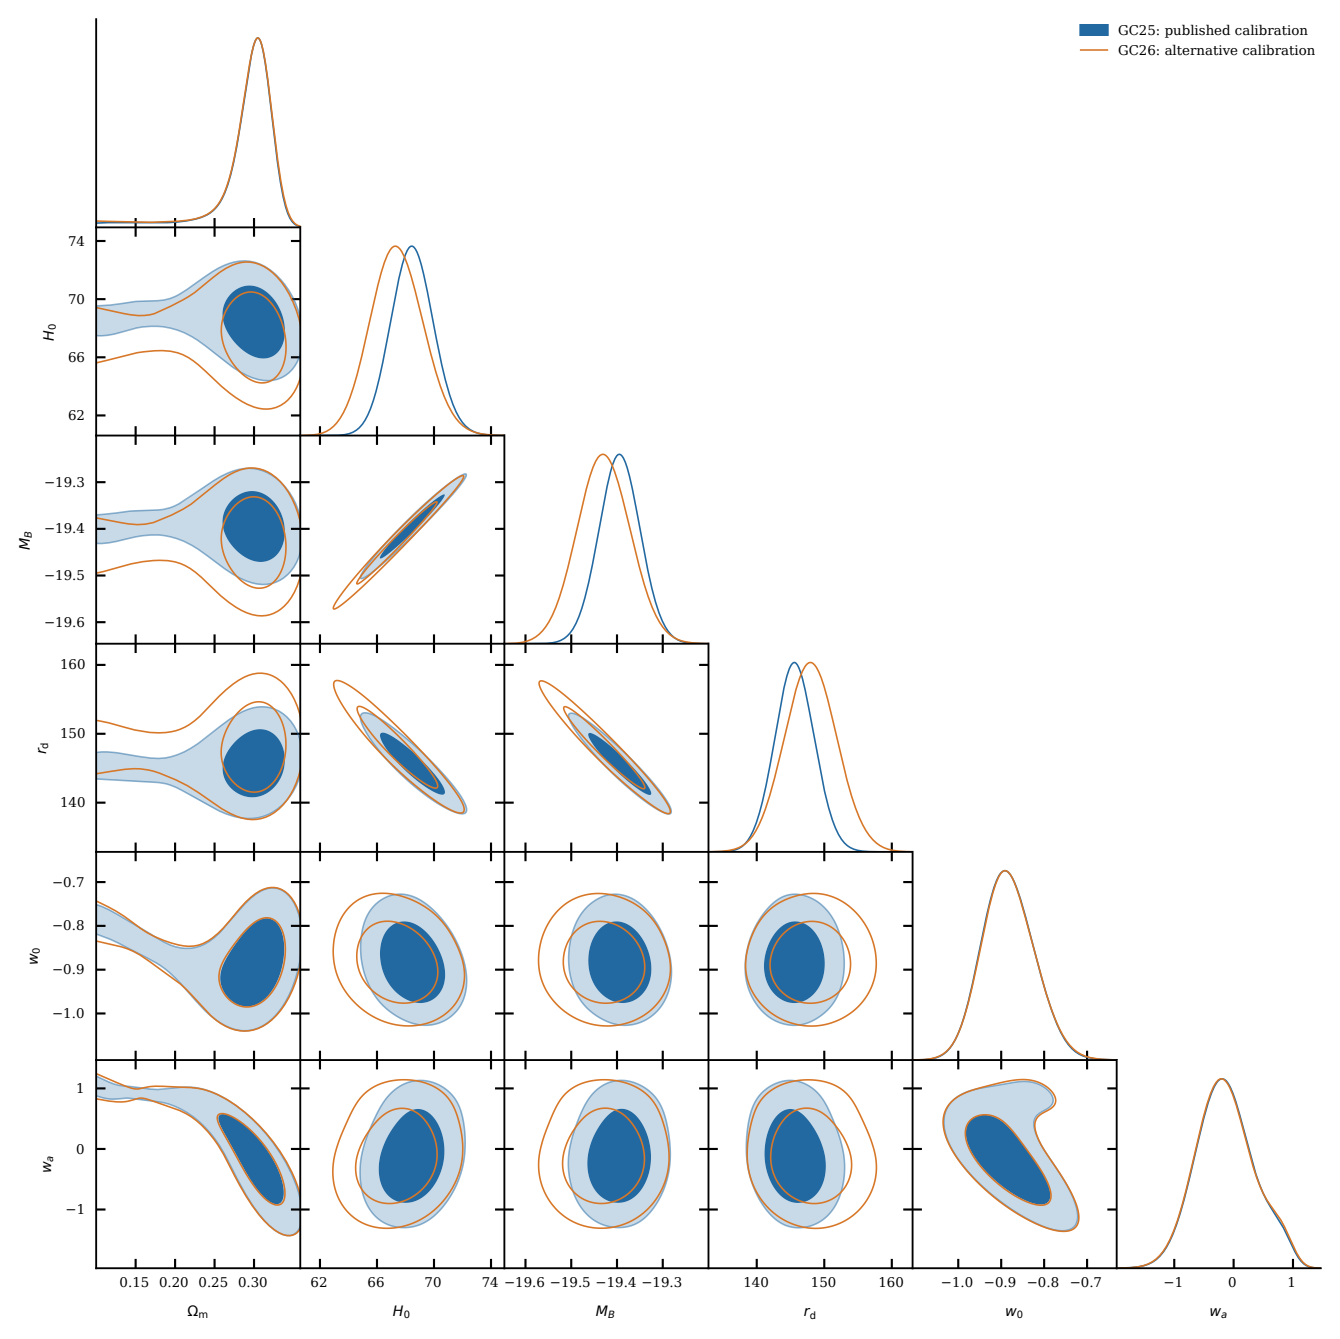

GC25: published calibration
GC26: alternative calibration
Ω_m
H_0
M_B
r_d
w_0
w_a