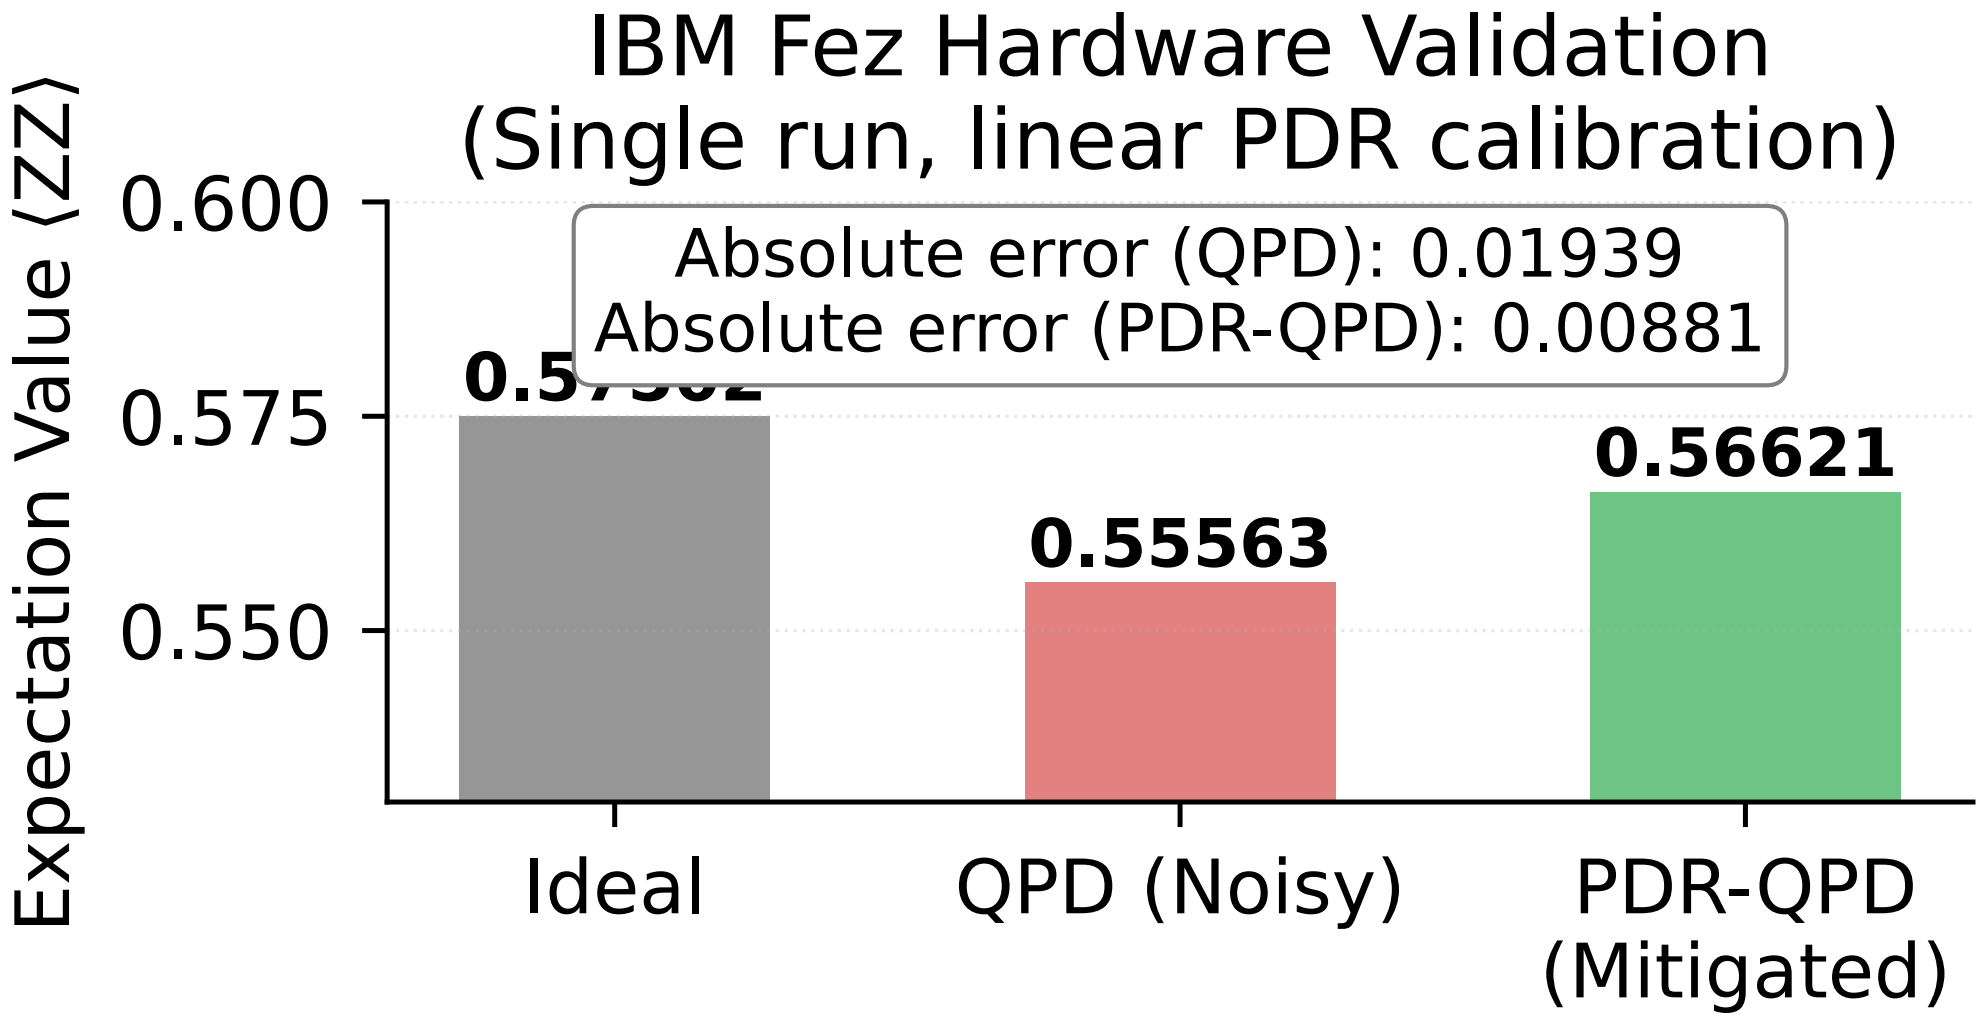
IBM Fez Hardware Validation
(Single run, linear PDR calibration)
Absolute error (QPD): 0.01939
Absolute error (PDR-QPD): 0.00881
Expectation Value ⟨ZZ⟩
0.600
0.575
0.550
0.55563
0.56621
Ideal
QPD (Noisy)
PDR-QPD
(Mitigated)