



Internal validation and clinical performance of OAI Model E


A. Participant-level cross-validated AUC

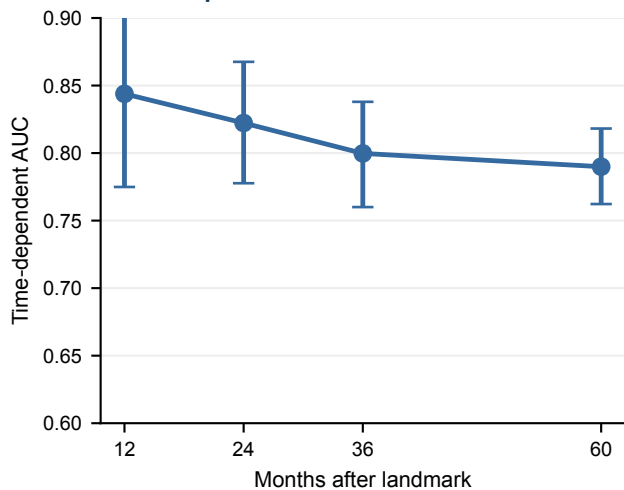


B. Participant-level 10-fold calibration

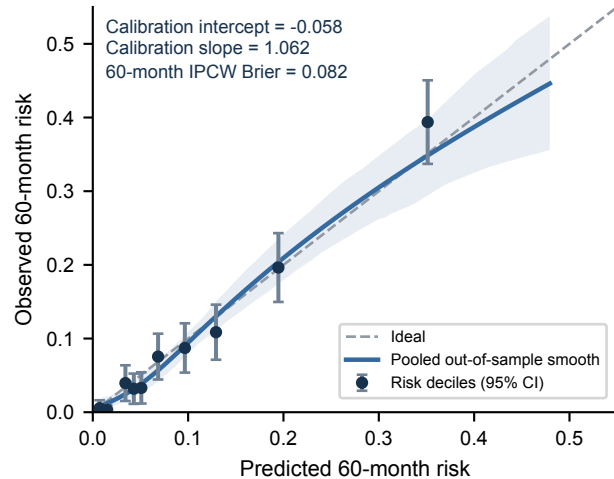

C. Decision-curve analysis at 60 months

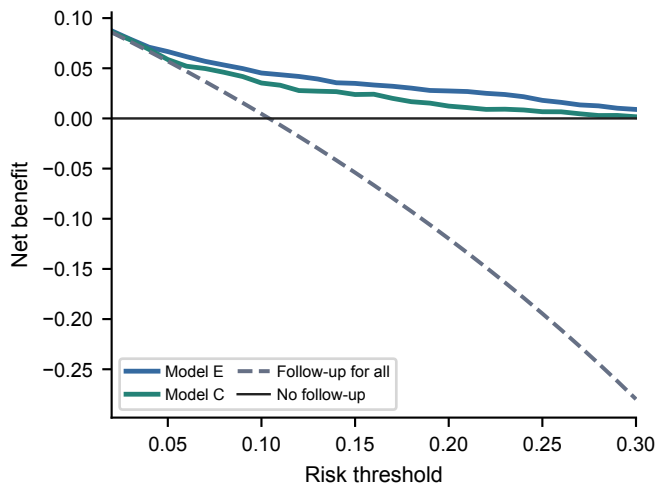

D. Risk by out-of-sample predicted-risk quartile

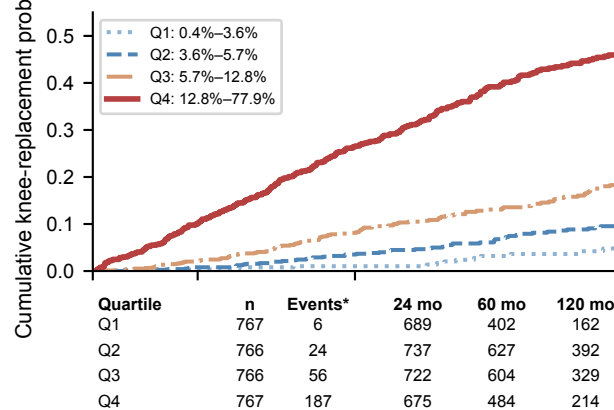

Panels A, B, and D use the same pooled participant-level 10-fold out-of-sample predictions.