


Data Analysis of PMS Data of Medical Devices

**Safety Signal Detection
(MAUDE DATA 2023)**


“Total number of incident reports

1048575


1. Safety Signal Detection

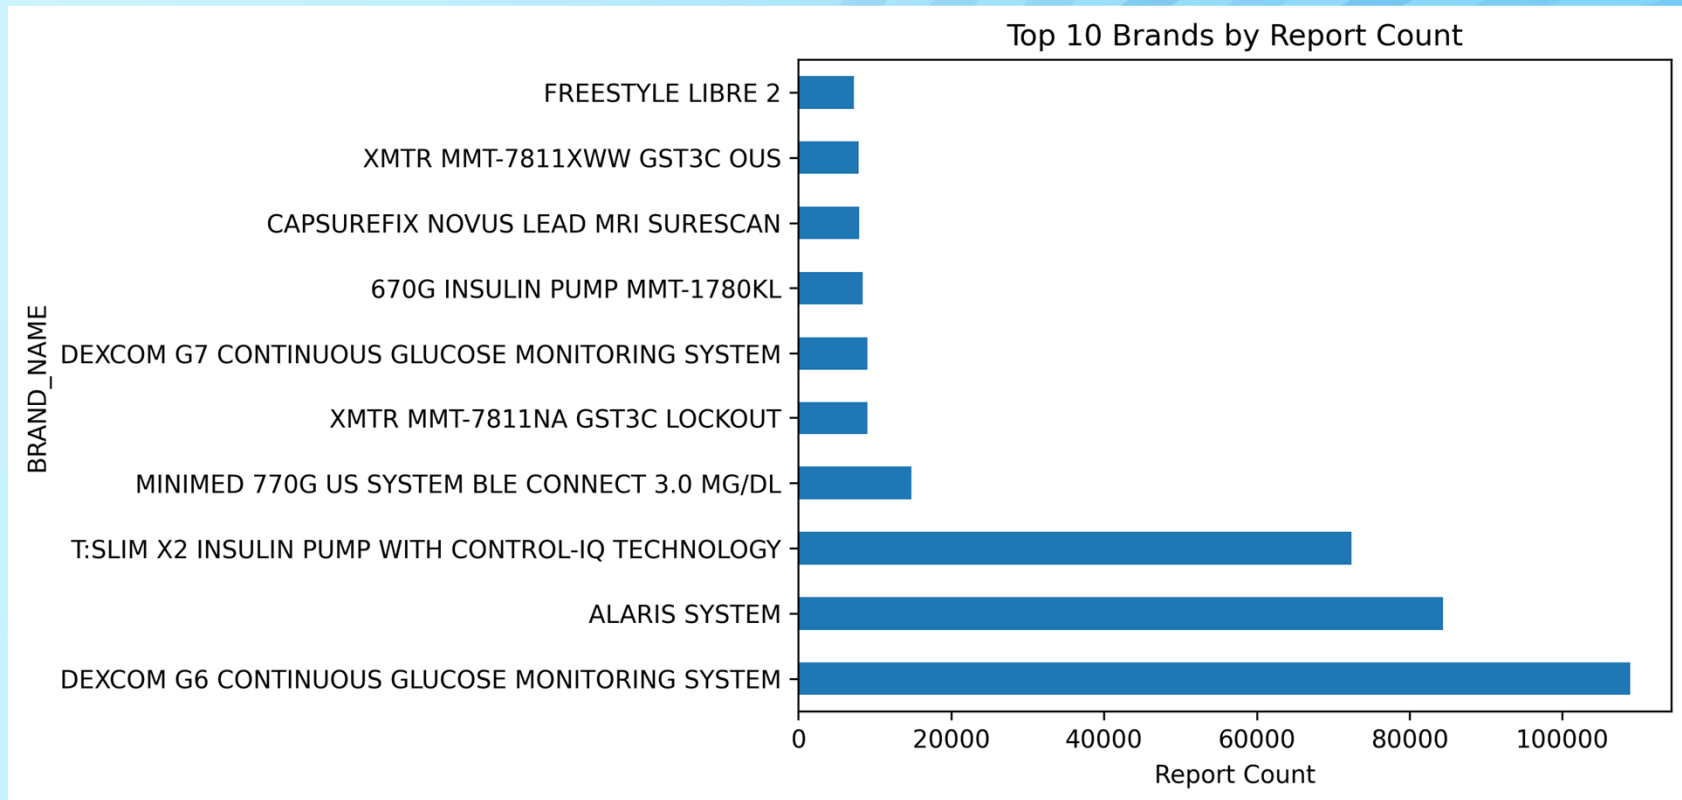

1. Safety Signal Detection

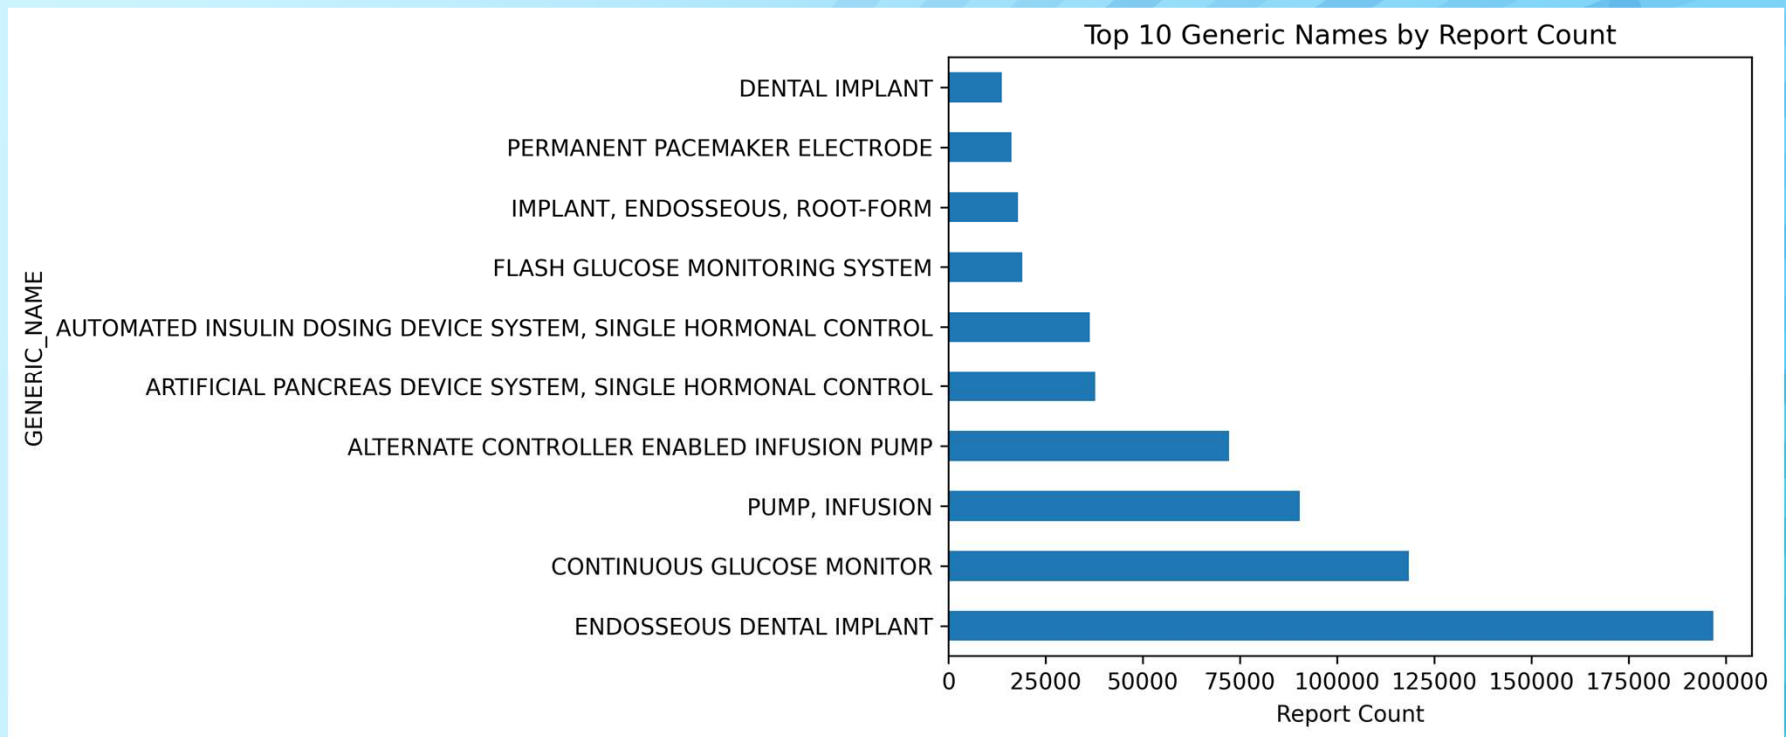

2. Time Trends

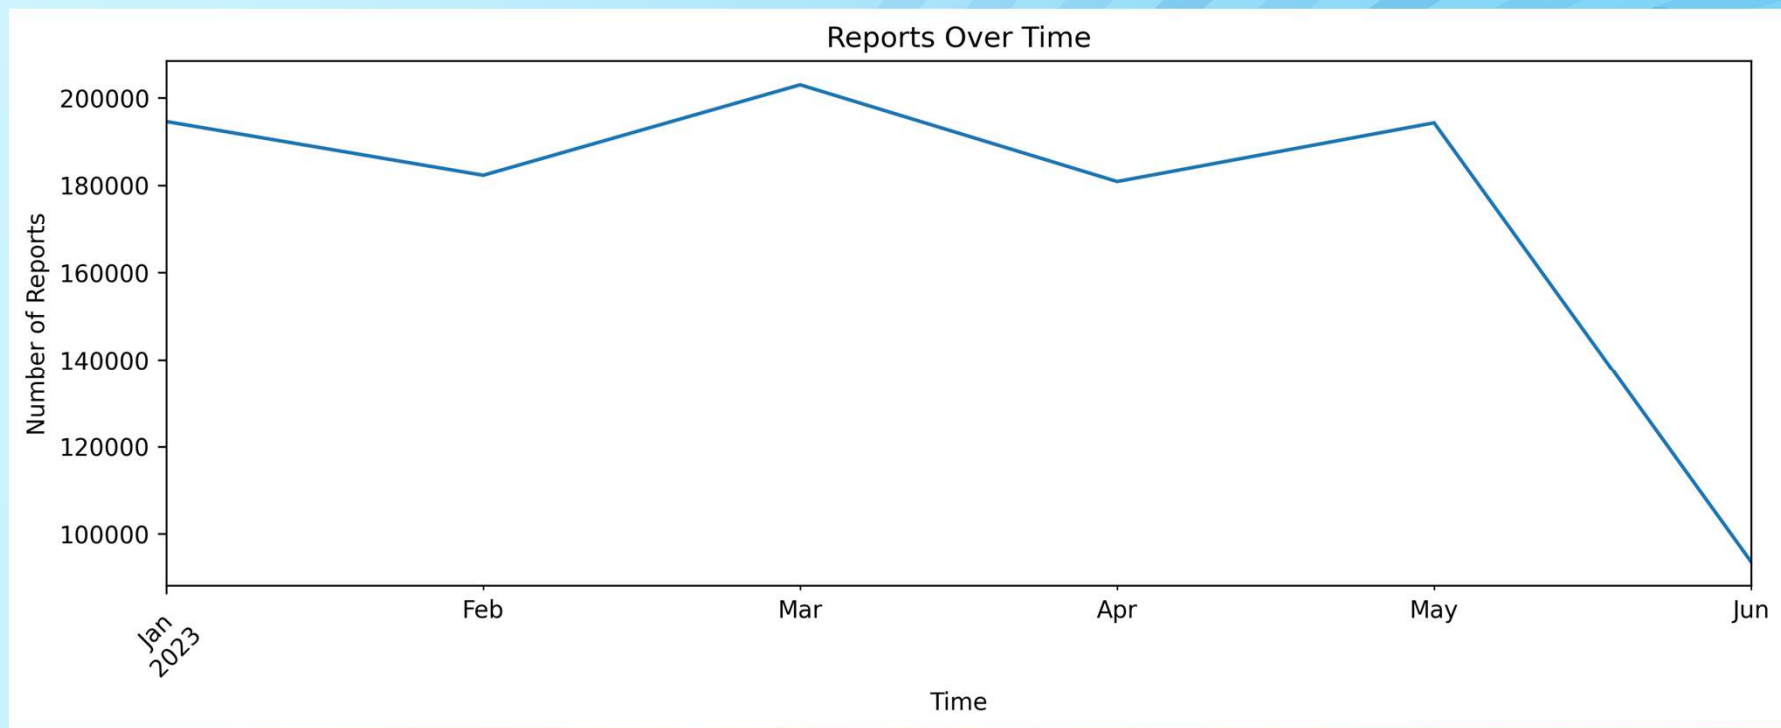




3. Device Usage Patterns

3. Device Usage Patterns

Implant Flag Distribution


OLYMPUS WINTER & IBE GMBH

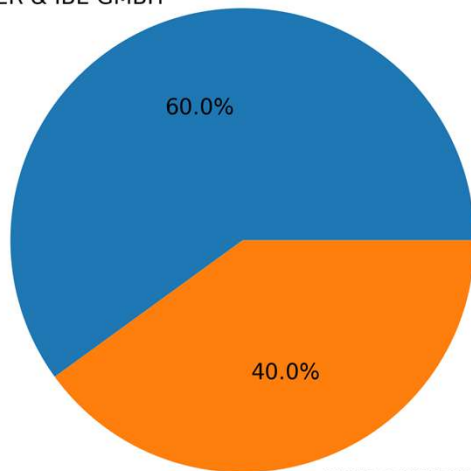

AIZU OLYMPUS CO., LTD.


Device Removed Flag Distribution

KUEHNSTRASSE 61

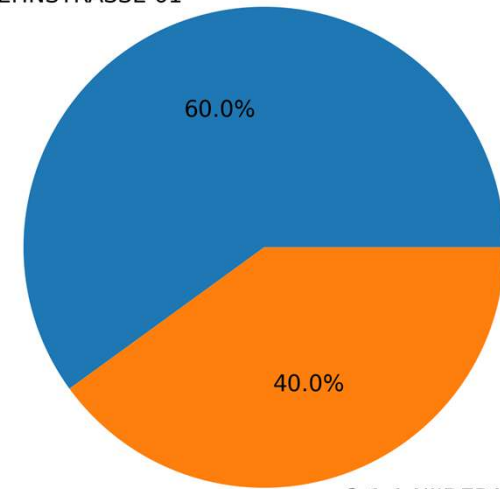


3-1-1 NIIDERAKITA



4. Manufacturer Performance

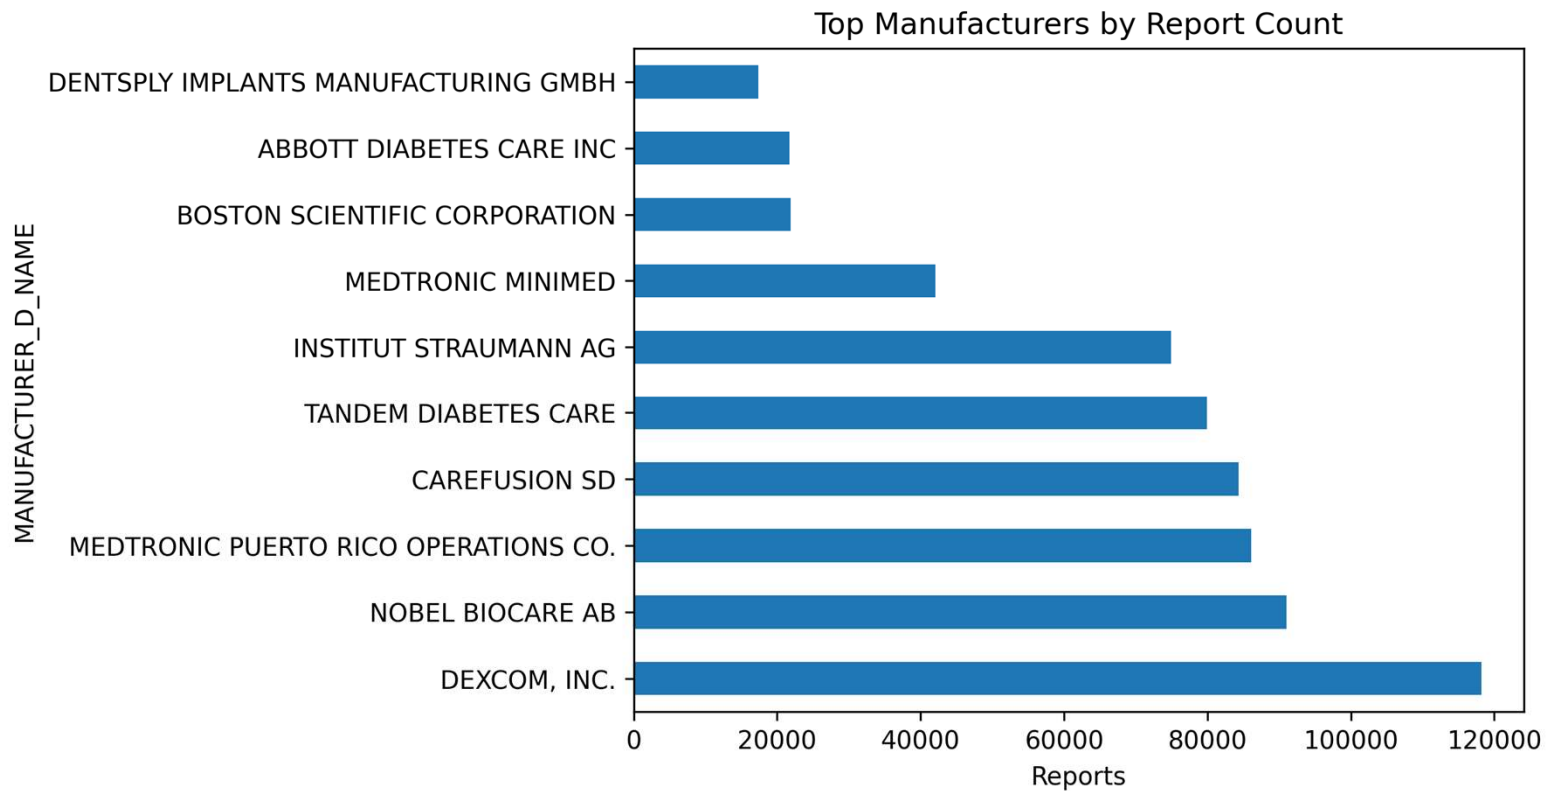


5. Product Code Analysis

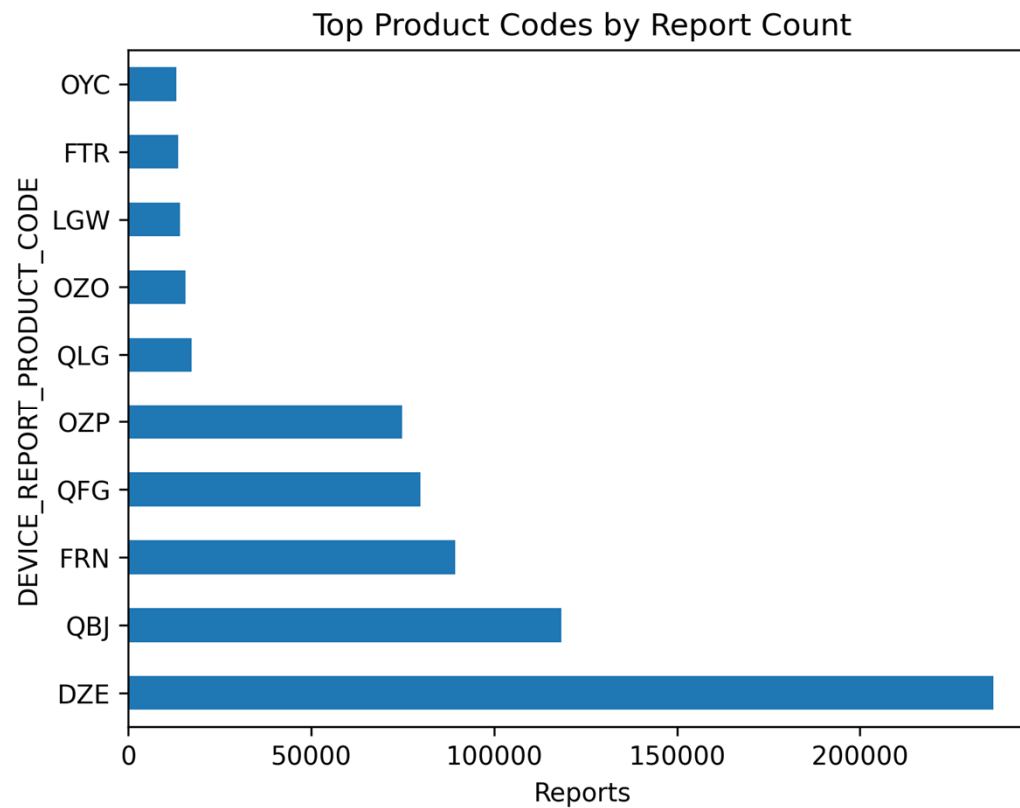



6. Return and Evaluation

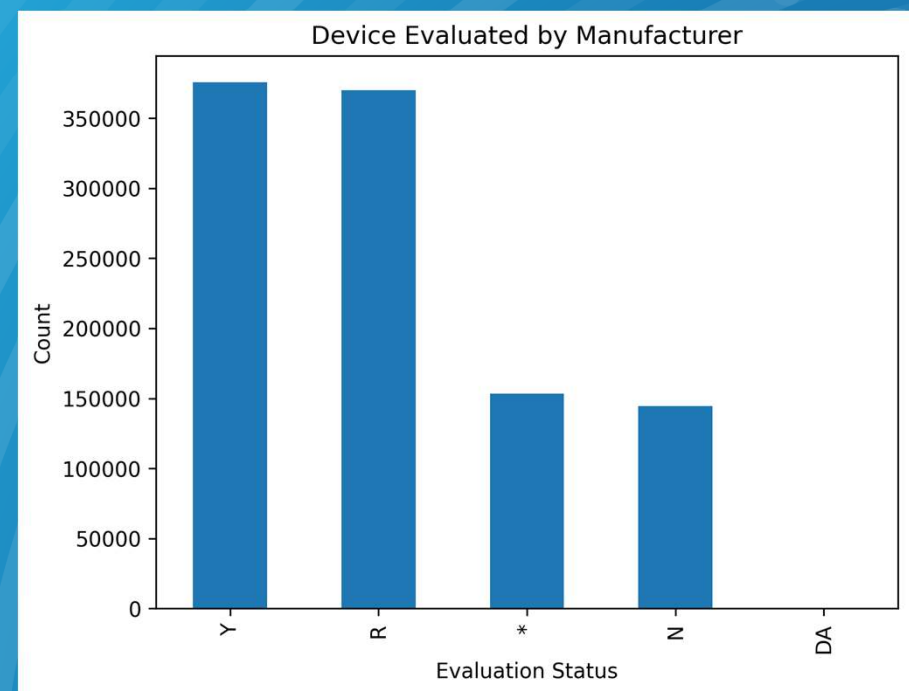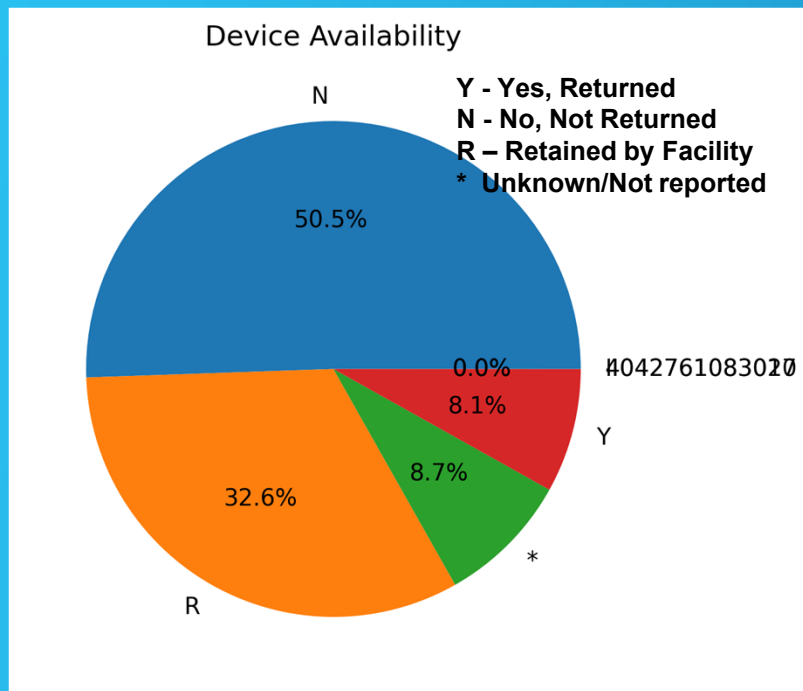




7. Combination Product Analysis

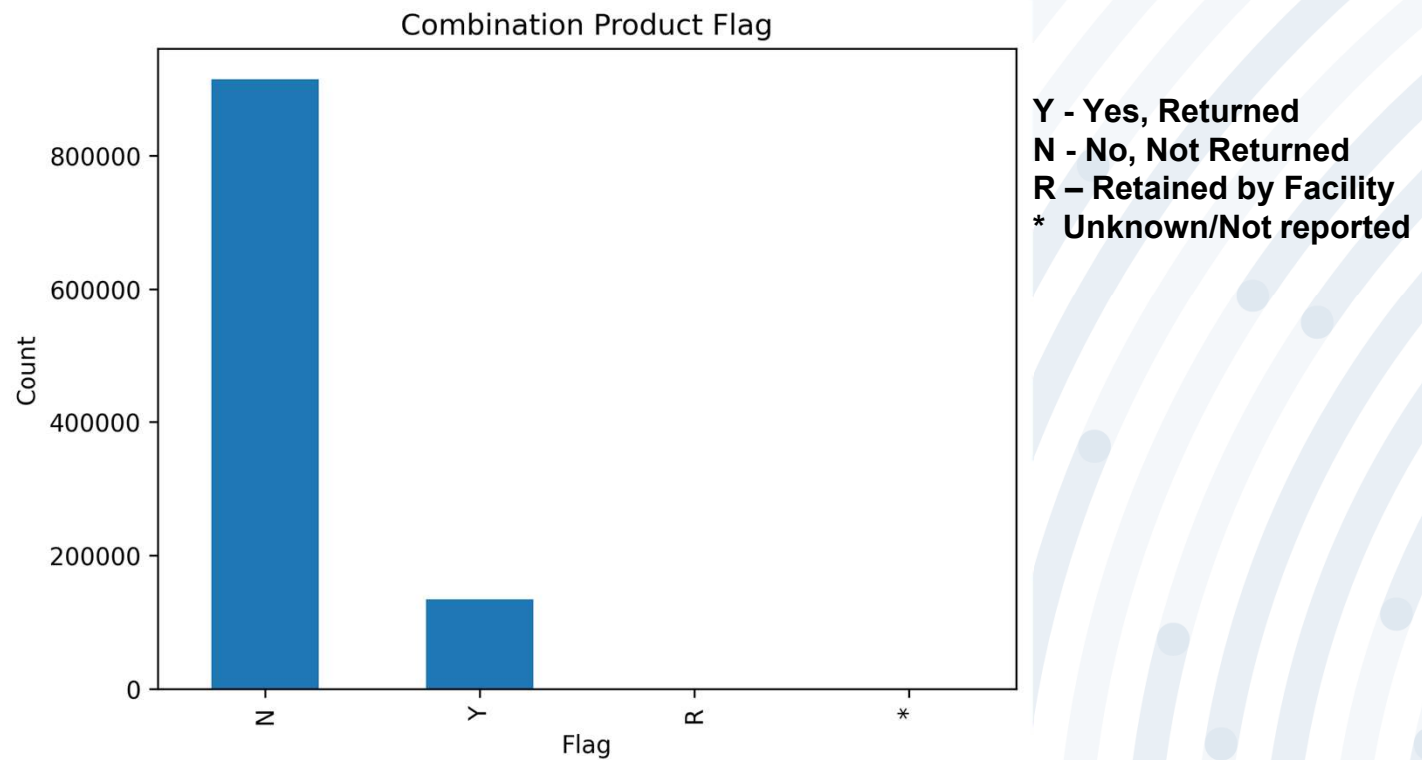

8. Temporal Trends

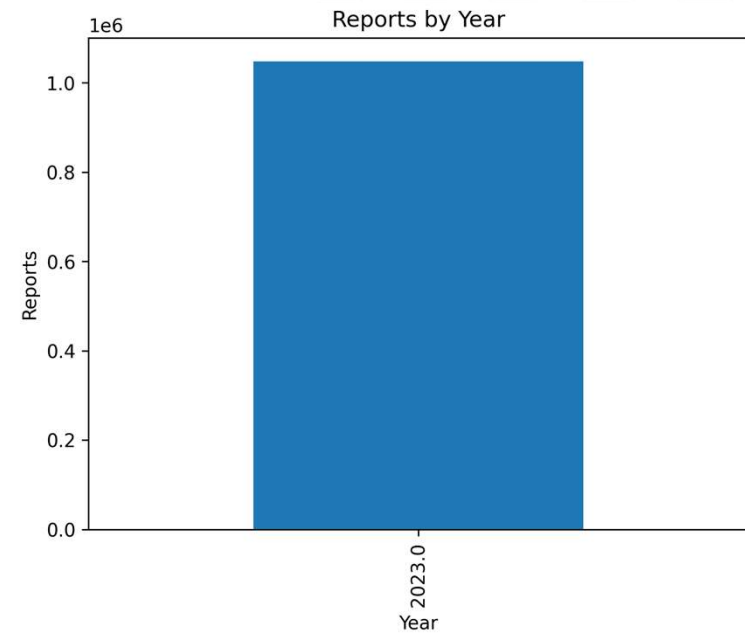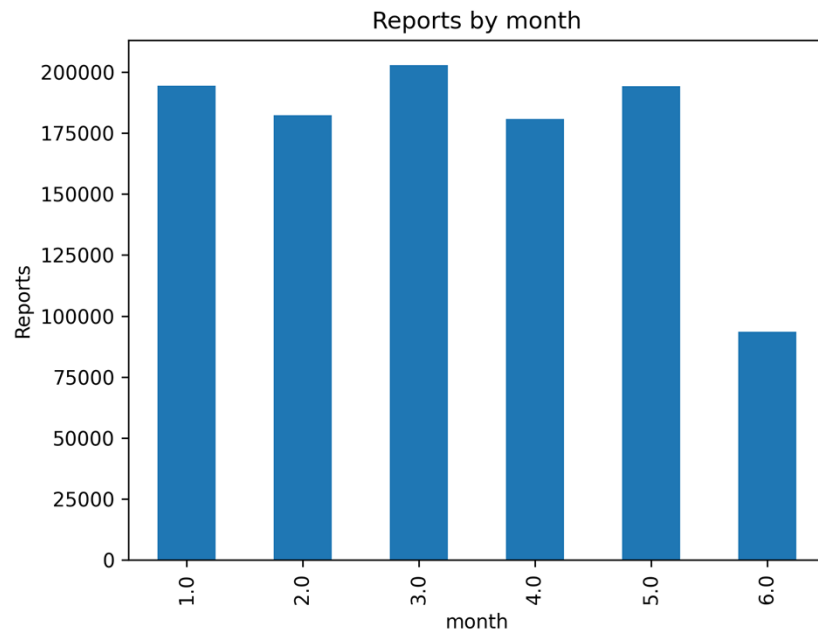

9. Regulatory & Risk Monitoring (Top 3)

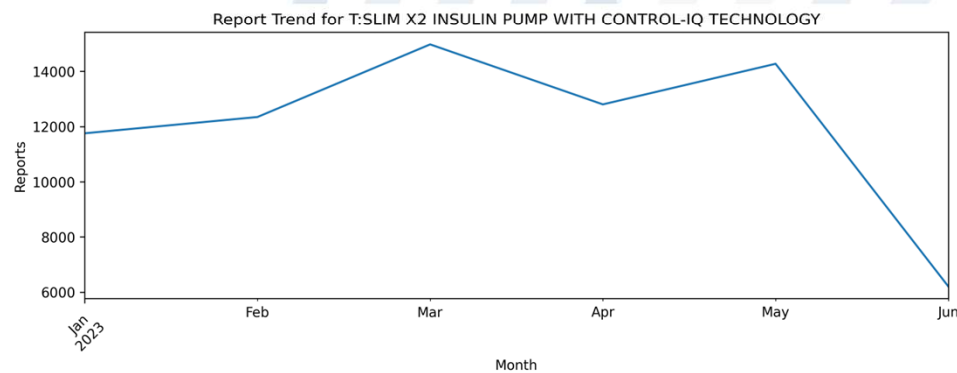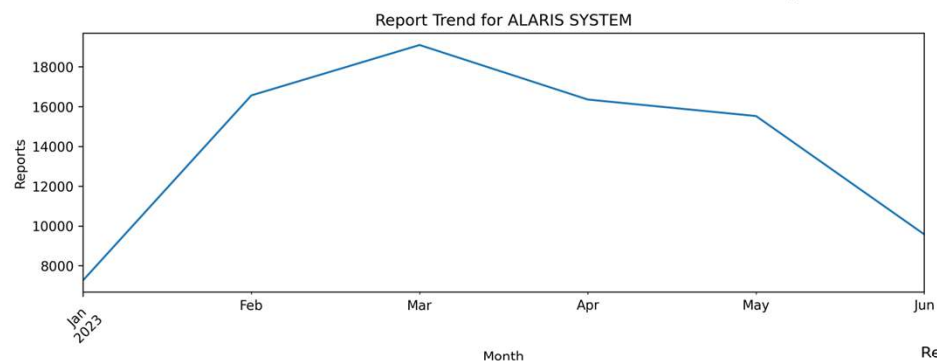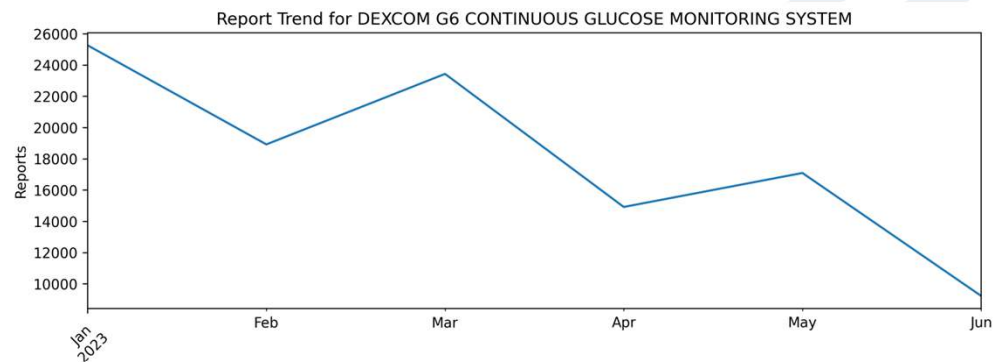

Summary

1. Brand Name with highest report count is
DEXCOM G6 CONTINUOUS GLUCOSE MONITORING SYSTEM
2. Brand Name with lowest report count is
FREESTYLE LIBRE 2

By -Hari Kamesh Kiran K

Summary

1. Generic Name with highest report count is
ENDOSSEOUS DENTAL IMPLANT
2. Generic Name with lowest report count is
DENTAL IMPLANT

By -Hari Kamesh Kiran K

Summary

1. Highest number of reports in **MARCH 2023**
2. Manufacturer with highest report count is **DEXCOM INC**
3. Manufacturer with lowest report count is **DENTSPLY IMPLANT**

By -Hari Kamesh Kiran K

For more DATA ANALYTICS

+ Follow

Linked in



By -Hari Kamesh Kiran K