

EXP-2024-047 — Hepatocyte Drug Screen A

Running · Day 7

Last sync: 12s ago

CELL VIABILITY

87%

-4% vs yesterday

DRUG EFFICACY SCORE

72/100

+3 since introduction

TEMPERATURE

37.0°C

Stable ±0.1°C


PH LEVEL

7.4

Within optimal range

Cell Viability Over Time

EXP-2024-047 · 7-day progression

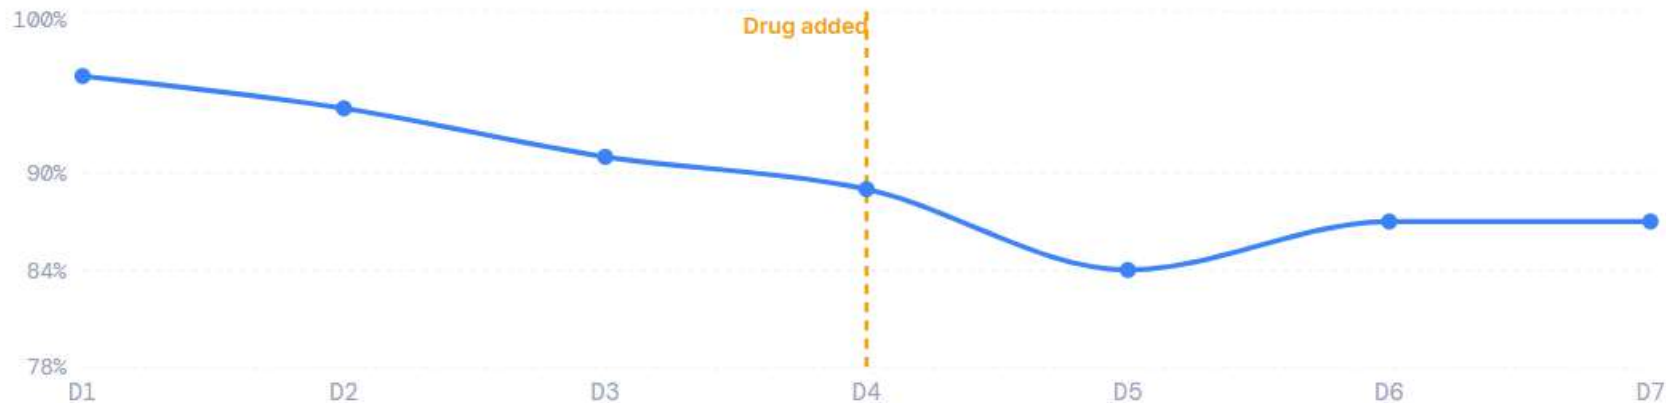

Live Sensor Feed

Live

Flow Rate 2.1 mL/min

Oxygen Level 19.8%

Glucose 4.2 mmol/L

Alert Feed

2 critical

Cell viability dropped below 90% threshold
2m ago

Flow rate deviation detected: ±0.3 mL/min
8m ago

Protocol Actions

Drag actions into the workflow

 Inject Drug A

 Wait 5 min

 Change Temperature

 Capture Image

 Increase Flow Rate

Workflow Builder

EXP-2024-047 · Protocol v3.2

1

 Inject Drug A


×

2

 Wait 5 min

×

Save Protocol

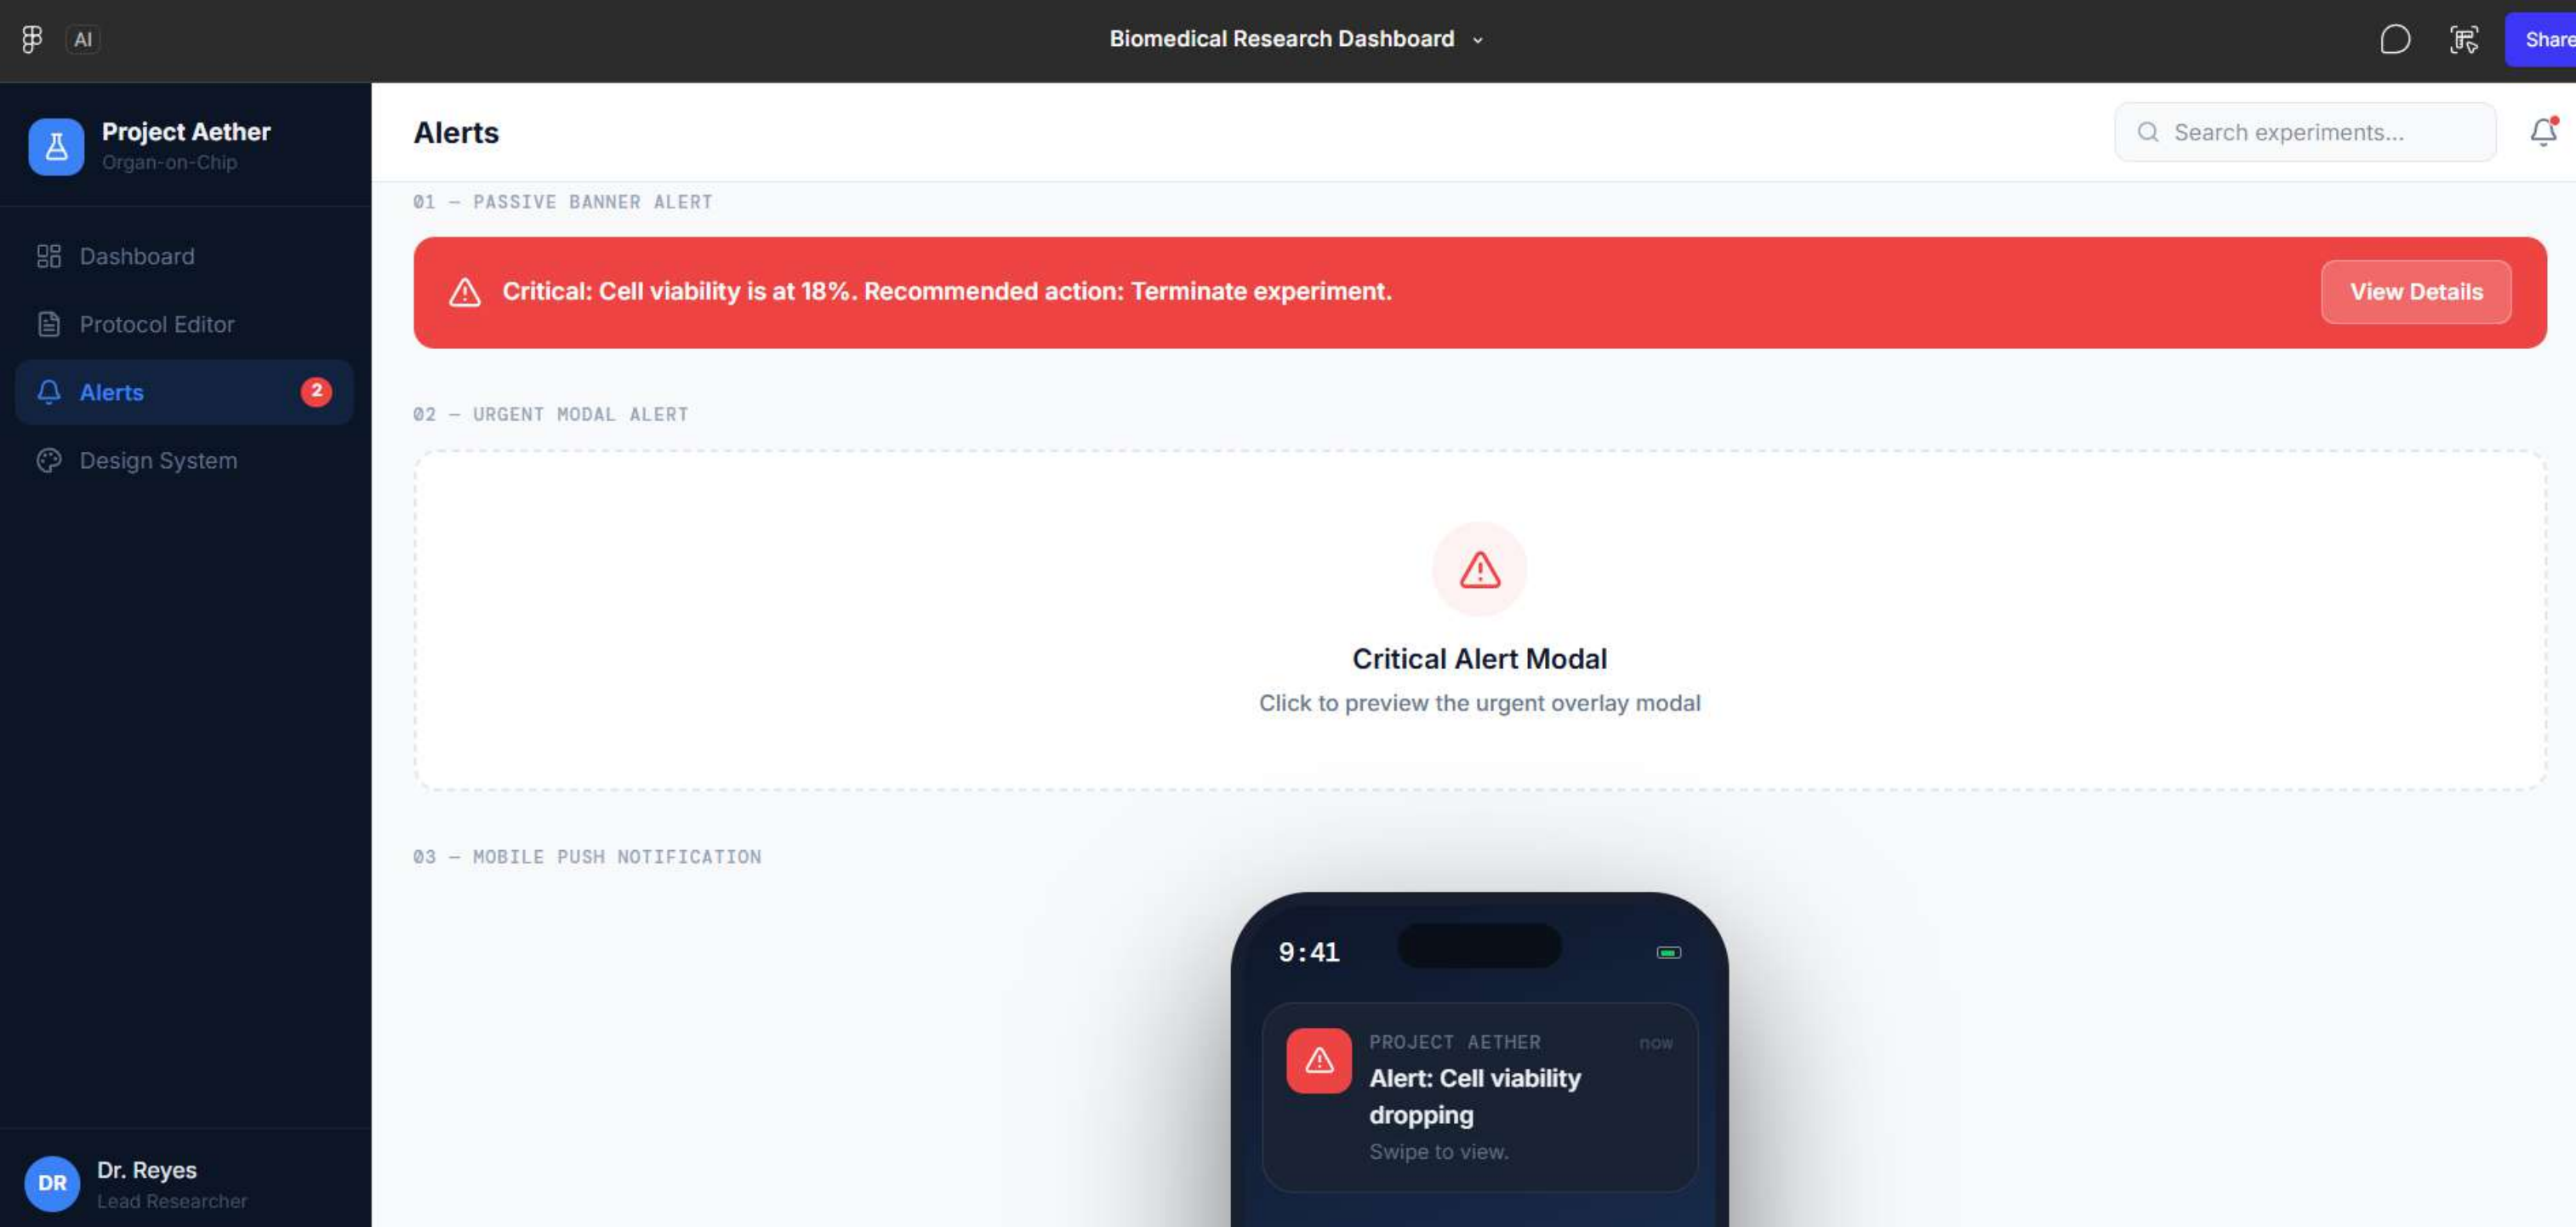

Design System

Q Search experiments...

Typography Scale

H1
32px - 700

Experiment Dashboard

H2
24px · 600

Cell Viability Analysis

BODY
16px • 400

Drug A injection completed at T+72h.

SMALL
14px - 400

Last sync: 12 seconds ago

MONO
13px - 500

87% · 37.0°C · 2.1 mL/min

Component Library

BUTTONS

Primary

Outlined

Danger

Ghost