Two stereo tone pairs in the first reference

32:48–33:18 excerpt · full 30-second Hann window · 0.033 Hz FFT bin spacing

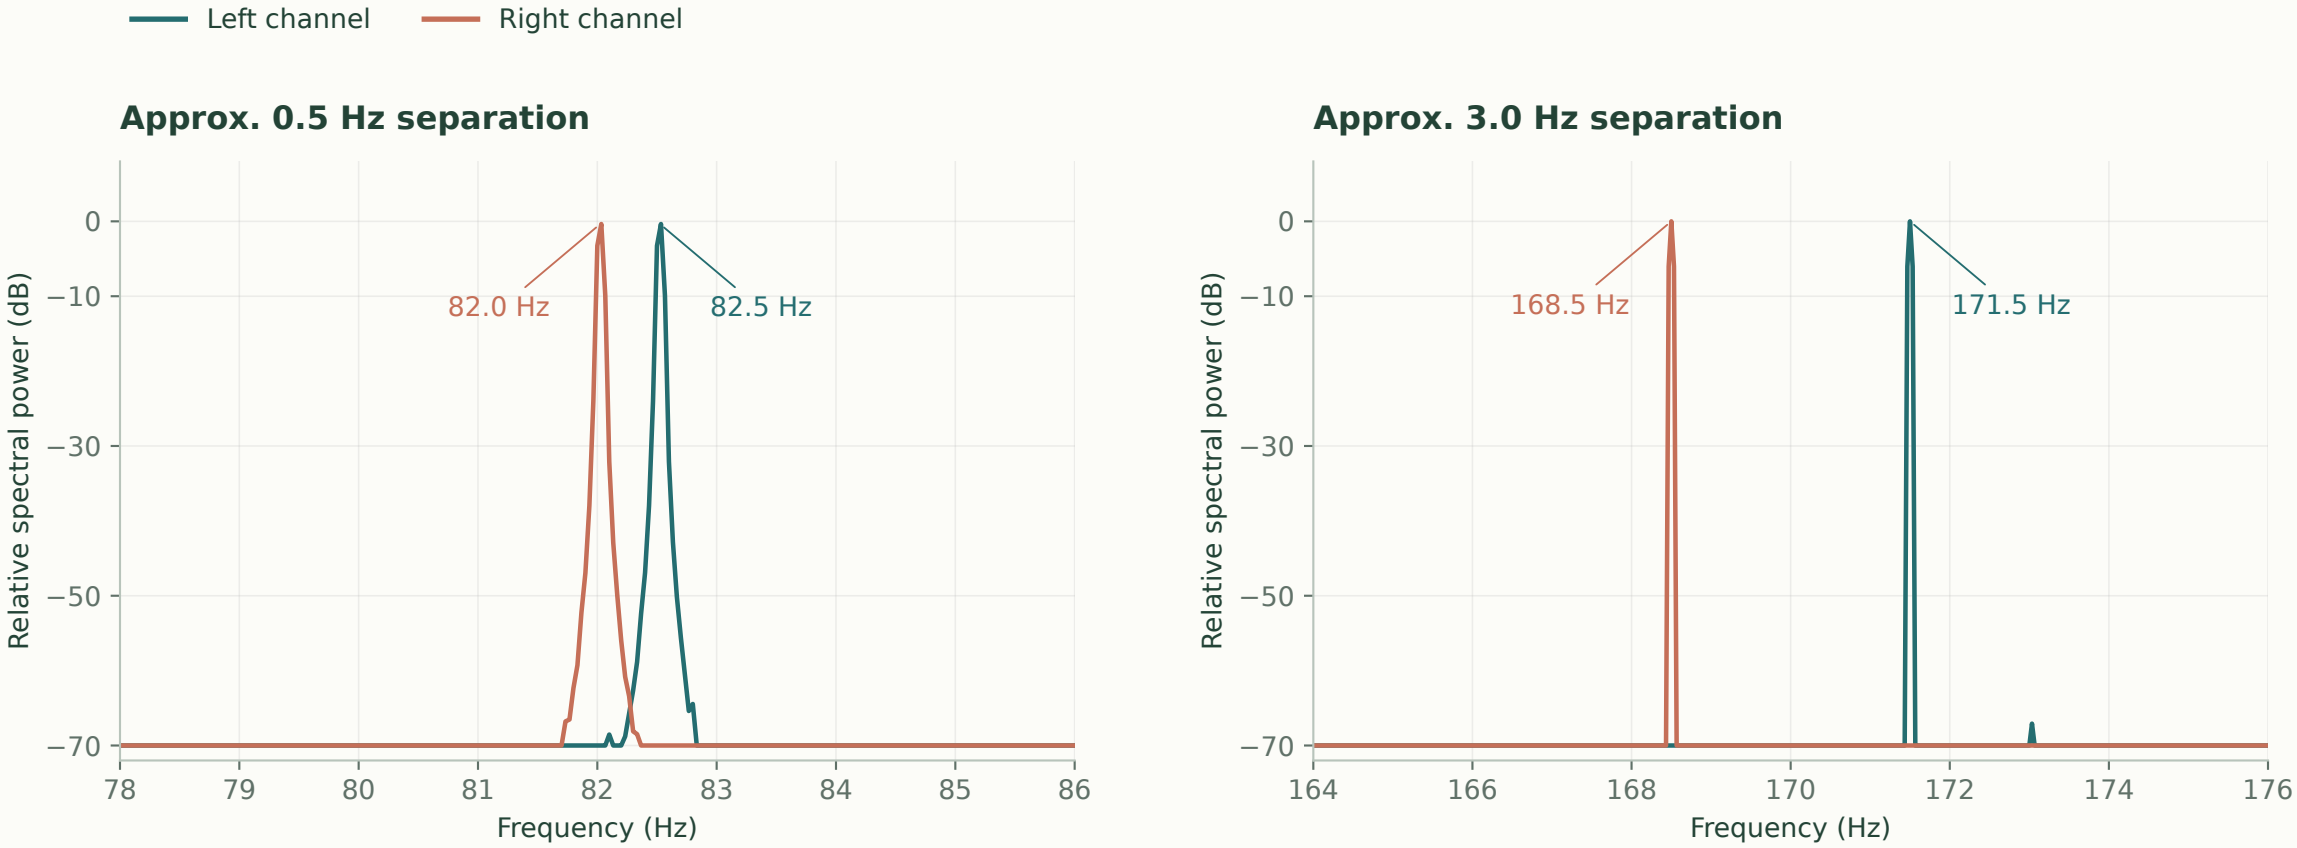

The two channels share one 0 dB reference. Rounded peak labels are shown; sub-bin estimates are not guaranteed resolving power.

The carrier frequencies and their differences are separate quantities. Ear-separated tones are compatible with binaural stimulation.

These measurements do not establish a perceived beat, brain entrainment, pain relief, or an effective treatment frequency.

Source: youtube.com/watch?v=fyGmSFUPo8o&t=1968s · Analysis limited to this excerpt.