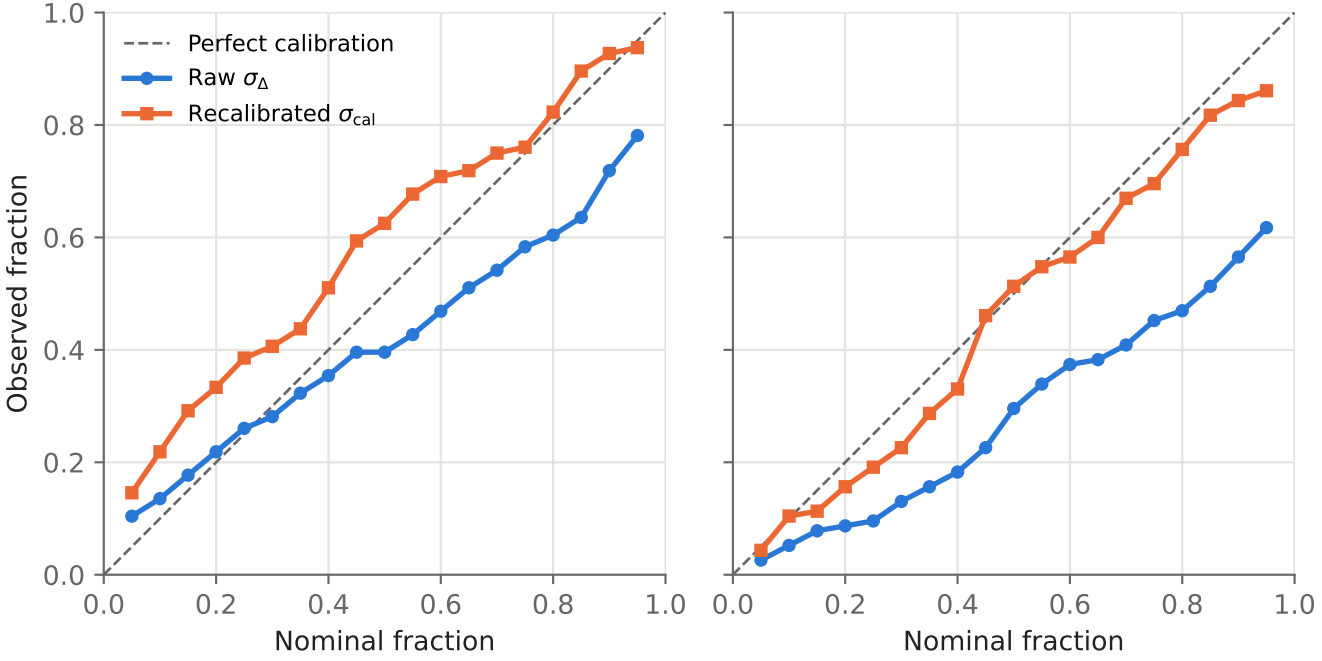
(A) Validation (n = 96)
(B) Held-out test (n = 115)
Perfect calibration
Raw σ_Δ
Recalibrated σ_{cal}
Observed fraction
Nominal fraction
Nominal fraction
0.0
0.2
0.4
0.6
0.8
1.0