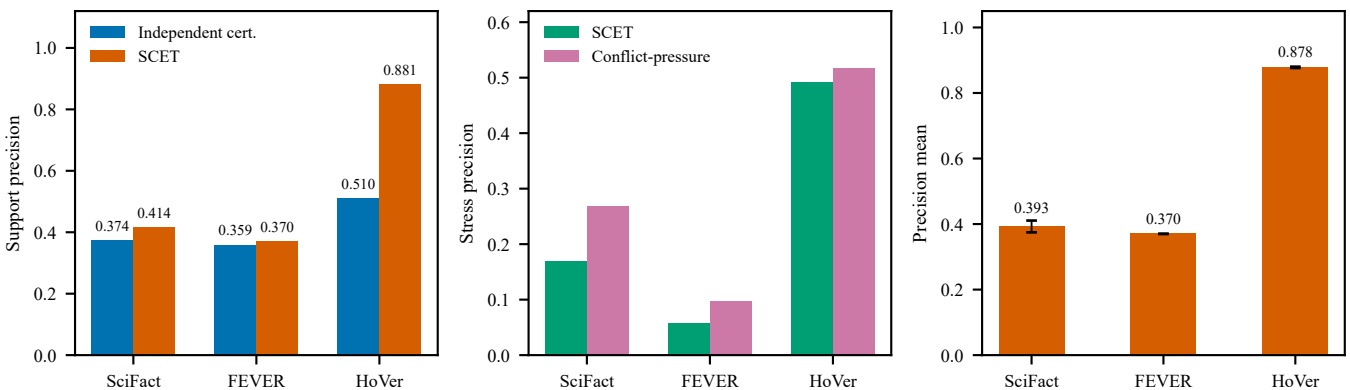
(a) Independent matched-volume
Independent cert.
SCET
Support precision
1.0
0.8
0.6
0.4
0.2
0.0
0.374
0.414
0.359
0.370
0.510
0.881
SciFact
FEVER
HoVer
(b) Conflict-pressure audit
SCET
Conflict-pressure
Stress precision
0.6
0.5
0.4
0.3
0.2
0.1
0.0
SciFact
FEVER
HoVer
(c) Calibration stability
Precision mean
1.0
0.8
0.6
0.4
0.2
0.0
0.393
0.370
0.878
SciFact
FEVER
HoVer