


PM100D, PM100A Firmware Update

- Check for an installed VISA version on your PC
- Install the 'DFU wizard' from the Tools folder on the memory stick
- Switch on the PM100 series device and browse the System Menu to Console Settings
- Enable the Firmware Upload (this feature disables automatically when turning off the unit)
- Connect the PM100 series device via USB cable to the PC
- PC will find a test and measurement device and a DFU device – please allow installing. A dialog box with several choices of drivers will appear. Please select 'DFU Capable Device (RUNTIME Mode)' from the path 'c:\windows\inf\thdfurun.inf':

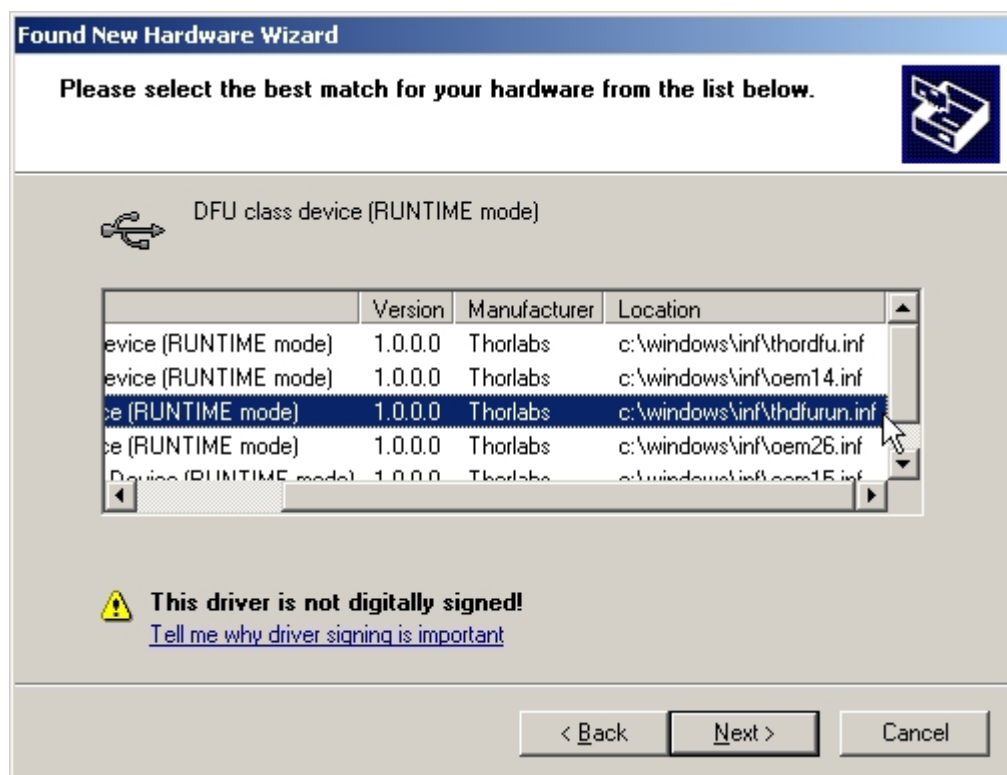

- Launch 'DFU wizard'
- Select the *.dfu file with the latest firmware version (included on memory stick or downloaded from our website)
- Press Next and Scan for DFU capable Devices

- The PC again will find a new USB device – allow installing, just clicking to ‘Next’ button.
- Press the Retry button in the wizard dialog box.
- The new firmware will install.
- DFU wizard will confirm then successful upload. In PM100A/D display may appear a hardware error message - please ignore it, switch off and on again the console - it will operate then normally.

Trouble Shooting:

The DFU wizard doesn’t find the connected PM100D/PM100A:

If the PM100 series device already was initialized as ‘test and measurement device’ on this PC and after enabling the Firmware Upload nothing happens – please check the device manager in the PC control panel. There might be a yellow exclamation mark by the test and measurement device. In this case give a right mouse click on the test and measurement device and allow updating the drivers. In case the updating doesn’t work, allow uninstall the driver. Perform a ‘search for new hardware’. From now on the procedure should work as described above.