

Edge Impulse credentials. Once logged in, a list of available devices will appear. Select the device created for health ML training. The

USB-connected board is detected automatically, and names must be assigned to the sensed values. In this case, the device sends two sets

of data: SpO₂ and heart rate, which are labelled as SpO₂ and HR. The device is now ready to upload data to Edge Impulse.

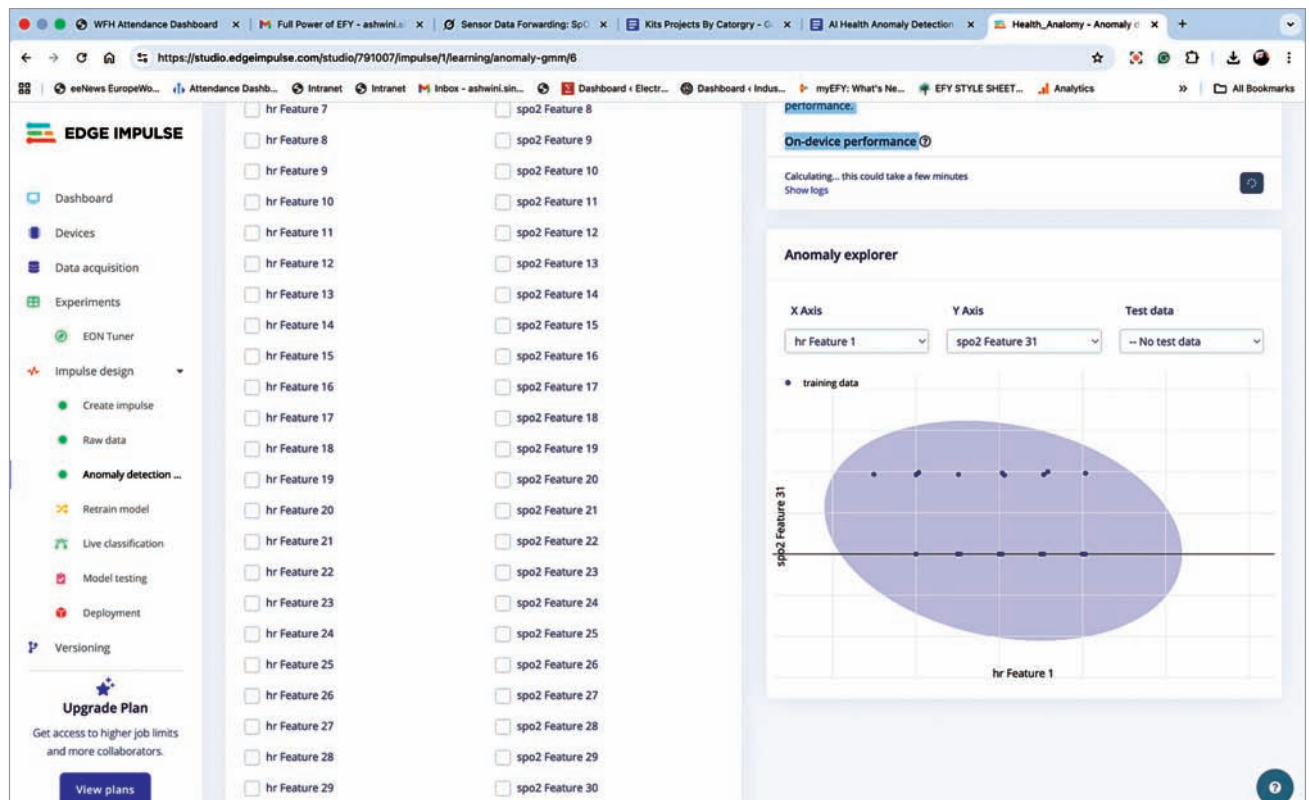


Fig. 5: Edge Impulse training ML model

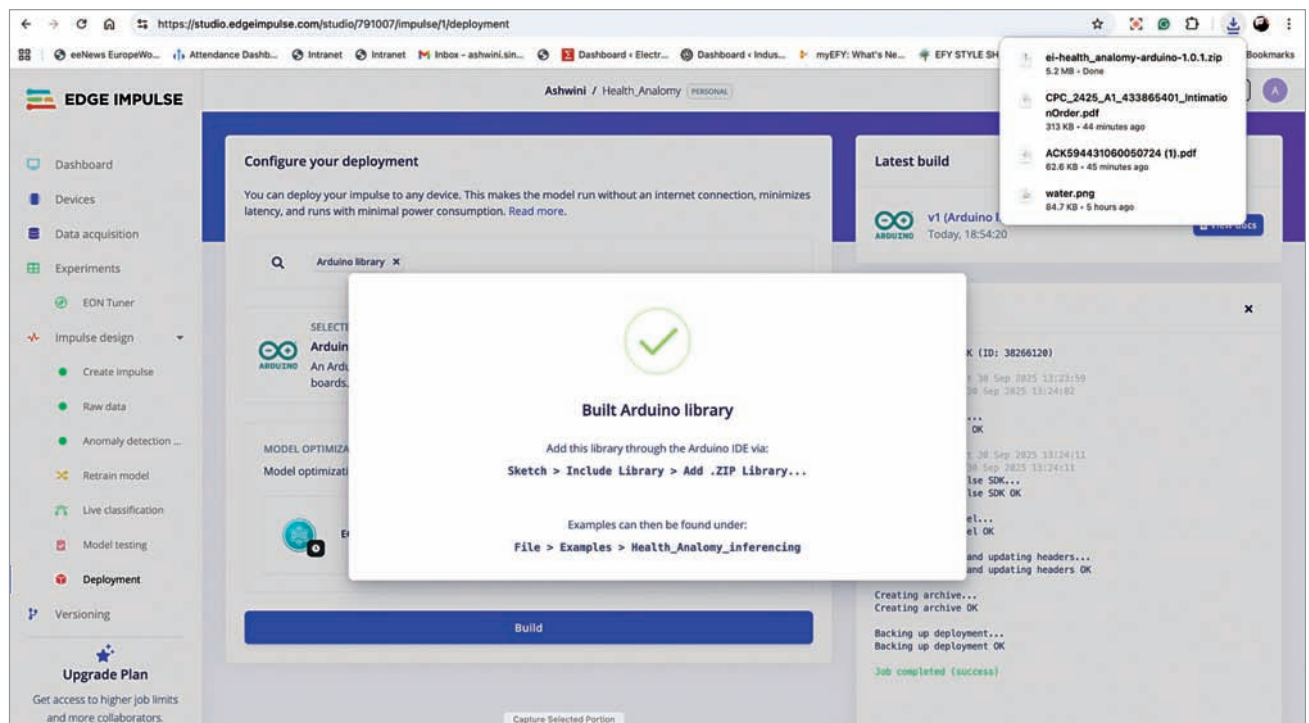


Fig. 6: Creating the ML model library for Arduino IDE