
Protocol for glucose estimation

S. No.	Reagents required	Blank B	Standard					Plasma	
			S1	S2	S3	S4	S5	T_1	T_2
1.	Standard glucose (ml)	-	0.5	1.0	1.5	2.0	2.5	-	-
2.	Concentration of glucose (µg)	-	50	100	150	200	250	-	-
3.	Test solution (ml)	-	-	-	-	-	-	0.5	1.0
4.	Distilled water (ml)	2.5	2.0	1.5	1.0	0.5	-	2.0	1.5
5.	Orthotoluidine reagent (ml)	4	4	4	4	4	4	4	4
Tubes are kept in boiling water for 20 minutes and cooled.									
6.	Optical density at 640nm								

Graph

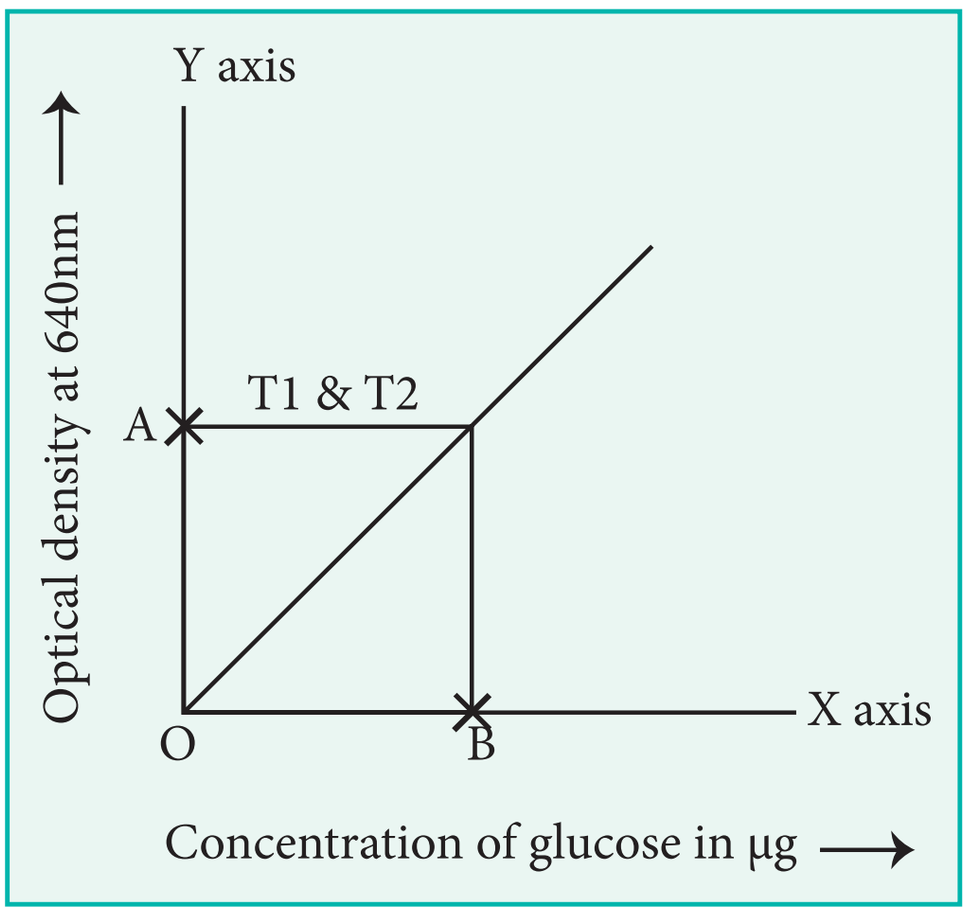

Practical_Bio-Chem-EM.indd 272 4/8/2020 3:28:52 PM