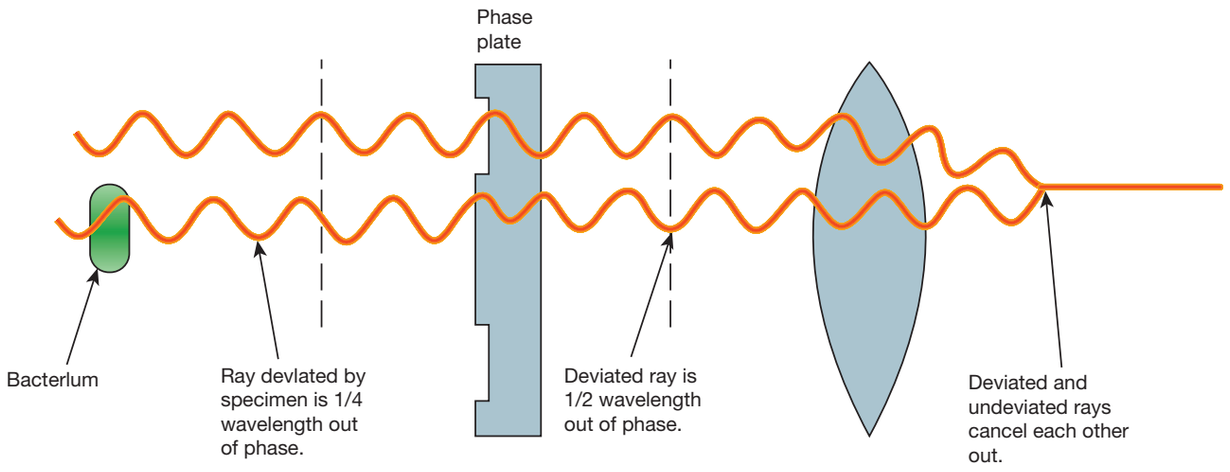


Figure 2.2: Production of contrast in phase contrast microscopy by phase plate

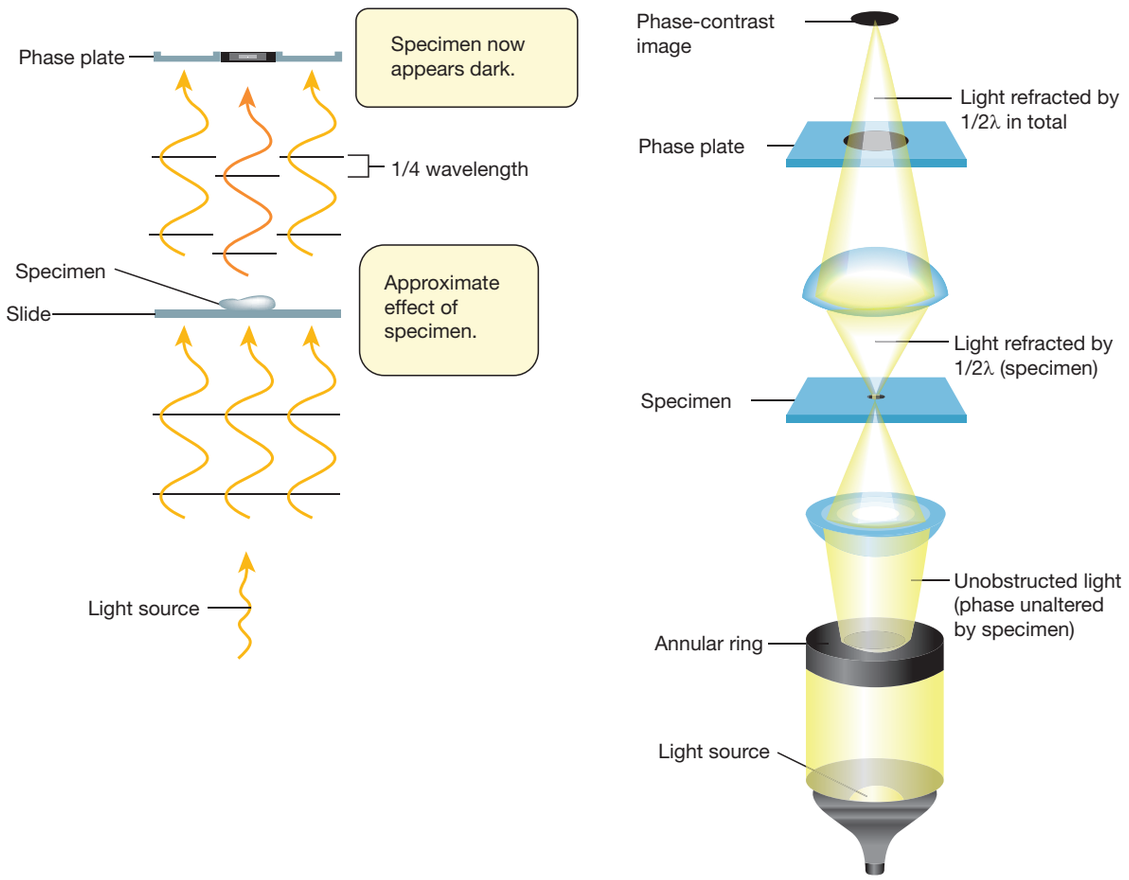


Figure 2.3: Optical path of Phase contrast microscopy

remain non-deviated (no phase change). Figure 2.3 shows the light path in phase contrast microscope.

HOTS

How does phase contrast microscope differ from Bright Field microscope?

TN_GOVT_XII_Micro_Biology_CH02.indd 14 27-02-2019 13:44:09