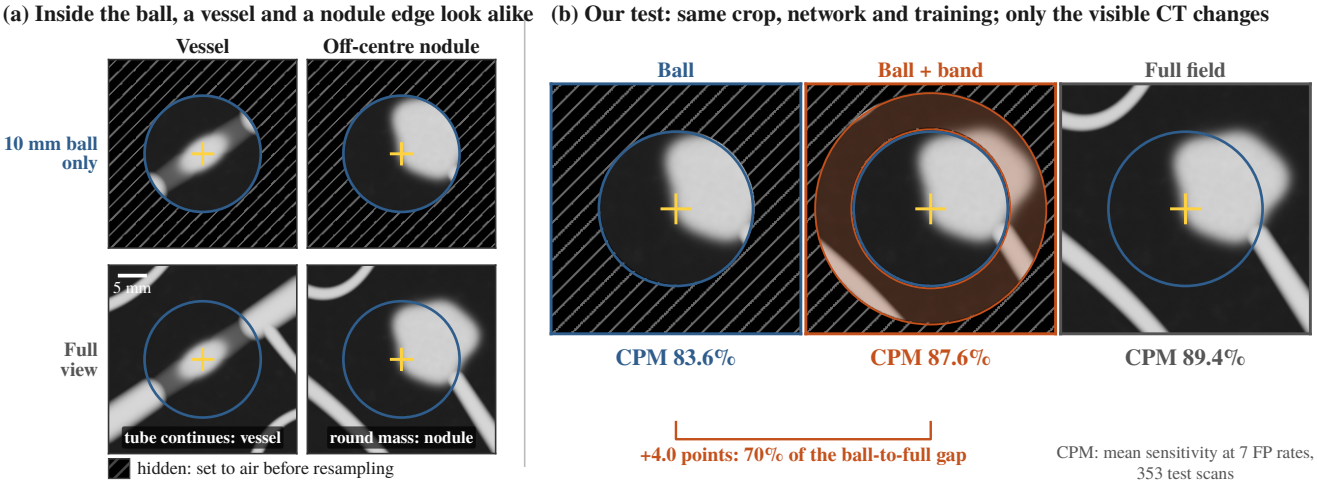

(a) Inside the ball, a vessel and a nodule edge look alike
Vessel
Off-centre nodule
10 mm ball only
Full view
5 mm
tube continues: vessel
round mass: nodule
hidden: set to air before resampling
(b) Our test: same crop, network and training; only the visible CT changes
Ball
Ball + band
Full field
CPM 83.6%
CPM 87.6%
CPM 89.4%
+4.0 points: 70% of the ball-to-full gap
CPM: mean sensitivity at 7 FP rates, 353 test scans