




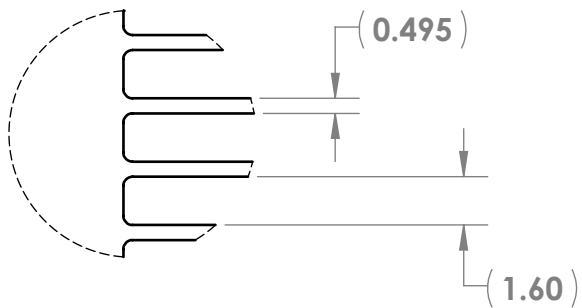

NOTE:  
THIS DOCUMENT CONTAINS CONFIDENTIAL AND PROPRIETARY  
INFORMATION OF CONFLUENT MEDICAL AND ALL DESIGN,  
MANUFACTURING, REPRODUCTION, USE AND SALE RIGHTS FOR  
SUCH INFORMATION ARE EXPRESSLY RESERVED.

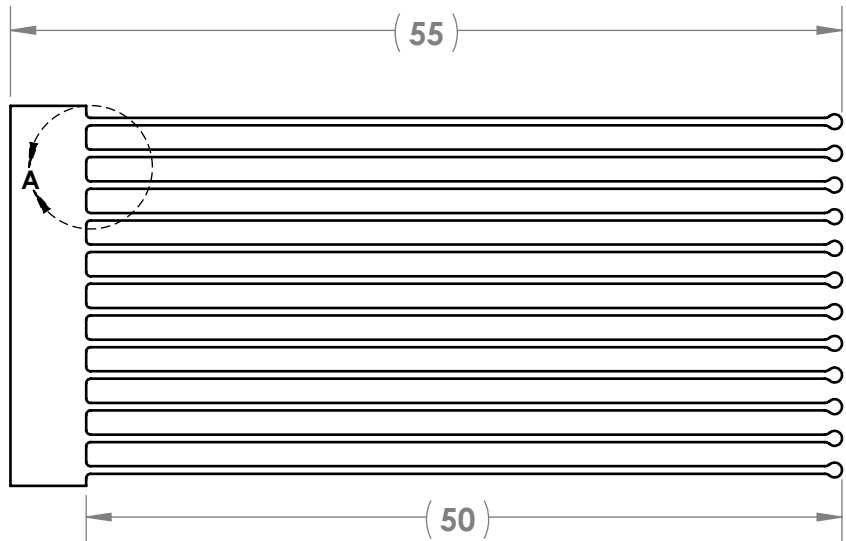

DETAIL A  
SCALE 4 : 1

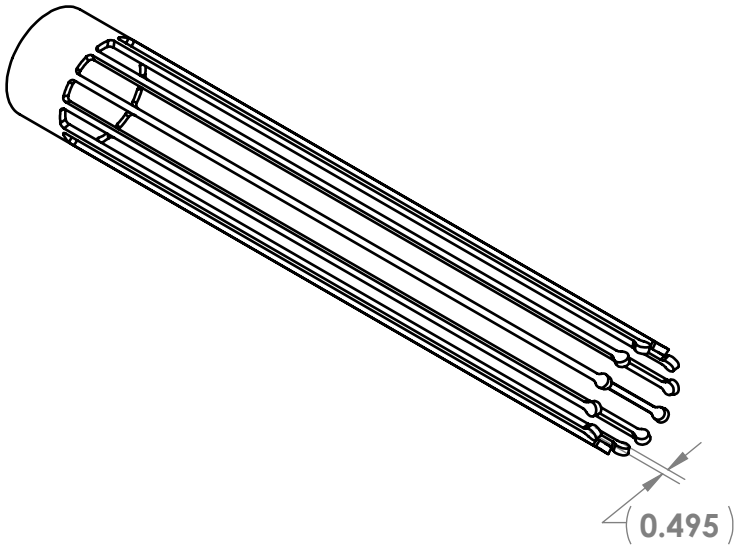

1. Laser cut according to specified pattern
2. Label with identifying details for source material and fabrication lot number

<b>CONFLUENT</b> MEDICAL TECHNOLOGIES		 <b>ndc</b> INTERFACE	DWG. TITLE: <b>Matchstick uCT samples 8.00x7.01 tubing</b>		
			SIZE: <b>B</b>	EPICOR NO:	
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS TOLERANCES ARE: 0 to 6 ± 0.1 OVER 6 TO 30 ± 0.2 OVER 30 TO 120 ± 0.3 OVER 120 TO 400 ± 0.5 OVER 400 ± 0.8 ANGLE ± 0.5°		THIRD ANGLE PROJECTION DESIGNED:  DATE:			PROJECT:
		DRAWN: <b>CB</b> DATE: <b>12/1/2016</b>		DWG NO: <b>NDC-03-06673</b>	REV: <b>1</b>
<> DIMS. INSPECTED PER NDC IP		n/a FILE NAME: NDC-03-06673 - R 11 SHEET: 1 OF 1			