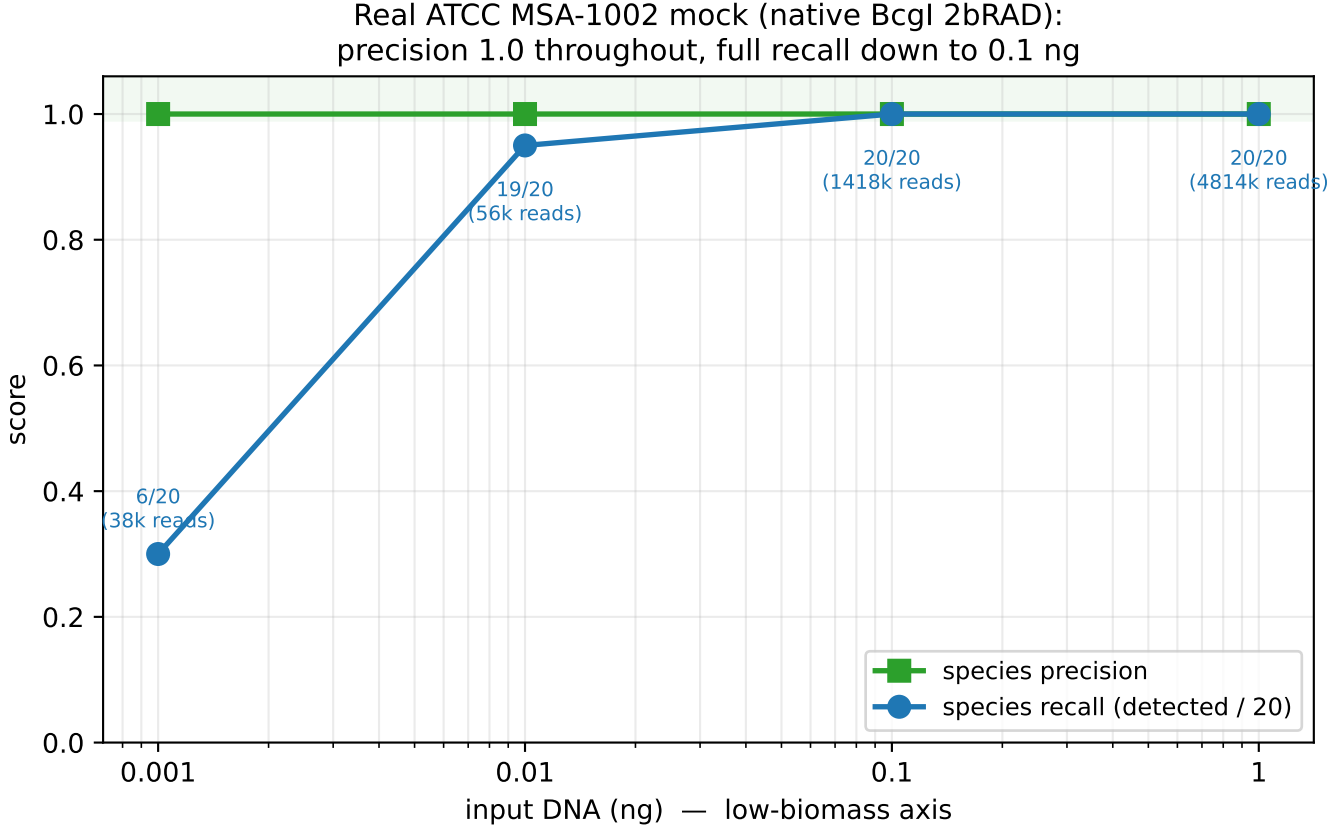
Real ATCC MSA-1002 mock (native BcgI 2bRAD):
precision 1.0 throughout, full recall down to 0.1 ng
score
1.0
0.8
0.6
0.4
0.2
0.0
6/20
(38k reads)
19/20
(56k reads)
20/20
(1418k reads)
20/20
(4814k reads)
species precision
species recall (detected / 20)
0.001
0.01
0.1
1
input DNA (ng) — low-biomass axis