



Syn2bANI calibrated ANI error is stable across GTDB-R207 genome quality


(a) CheckM completeness (min of pair)

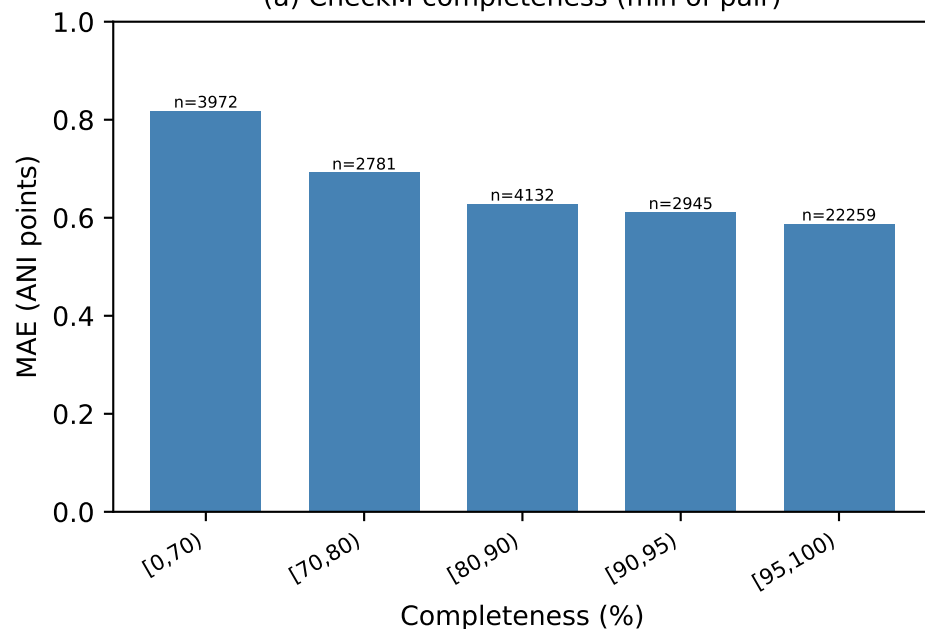

(b) CheckM contamination (max of pair)

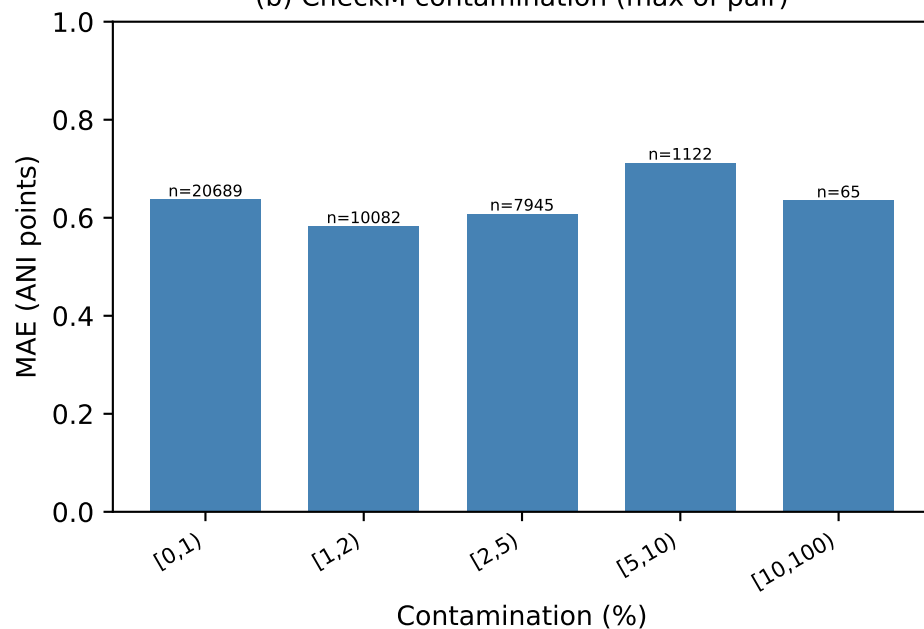

(c) Contig count (max of pair)

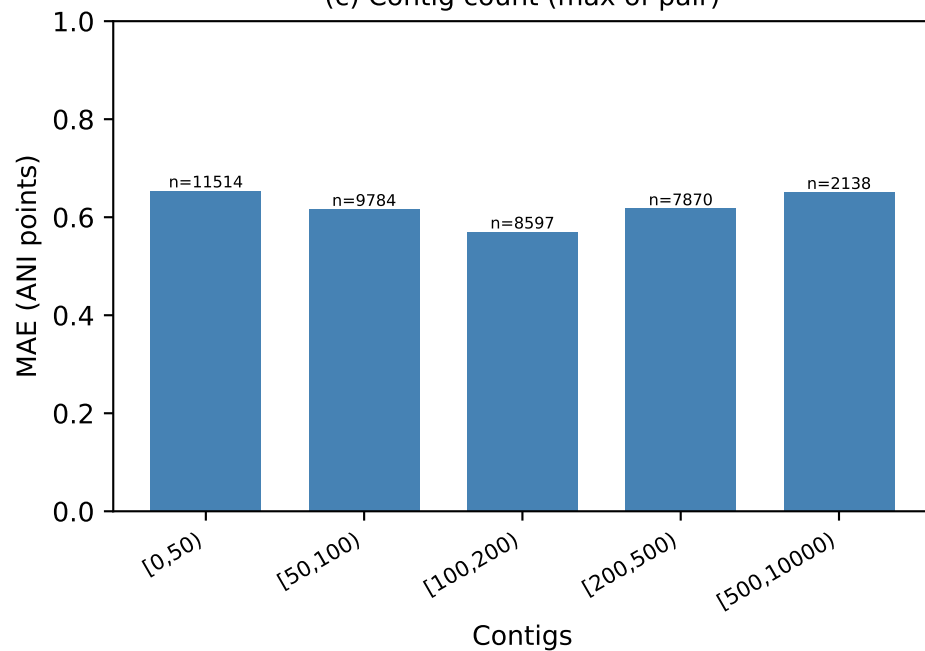

(d) Mean contig length (min of pair)

