Project Development Phase
Model Performance Test

Date	10 November 2022
Team ID	PNT2022TMID52879
Project Name	Classification Of Arrhythmia By Using Deep Learning With 2-D ECG Spectral Image Representation
Maximum Marks	10 Marks

Model Performance Testing:

S.No.	Parameter	Values	Screenshot
1.	Model Summary	-	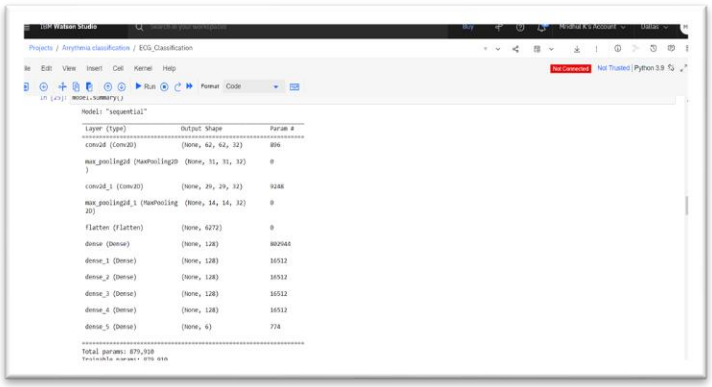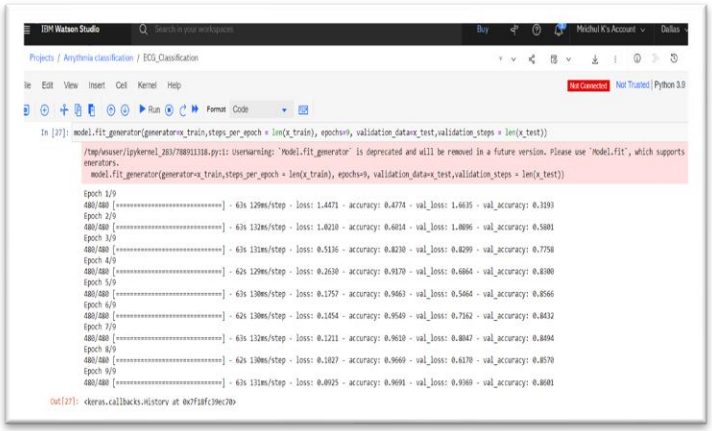
2.	Accuracy	Training Accuracy - 96.91% Validation Accuracy - 86.01%