


Sample Name: 397-U1586A-1H-5-HS

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : NGA-2                      Location :    1 (F)
Injection Date  : 10/17/2022 12:51:19 PM
                                           Inj Volume : Manual ly
Method          : C:\CHEM32\2\METHODS\397_NGA2_FID_ONLY.M
Last changed    : 10/14/2022 10:46:20 AM by SYSTEM
                  (modified after loading)
Method Info     : manual headspace injections

Sample Info     : CYL11739111
=====
```

Sample-related custom fields:

Name	Value
------	-------

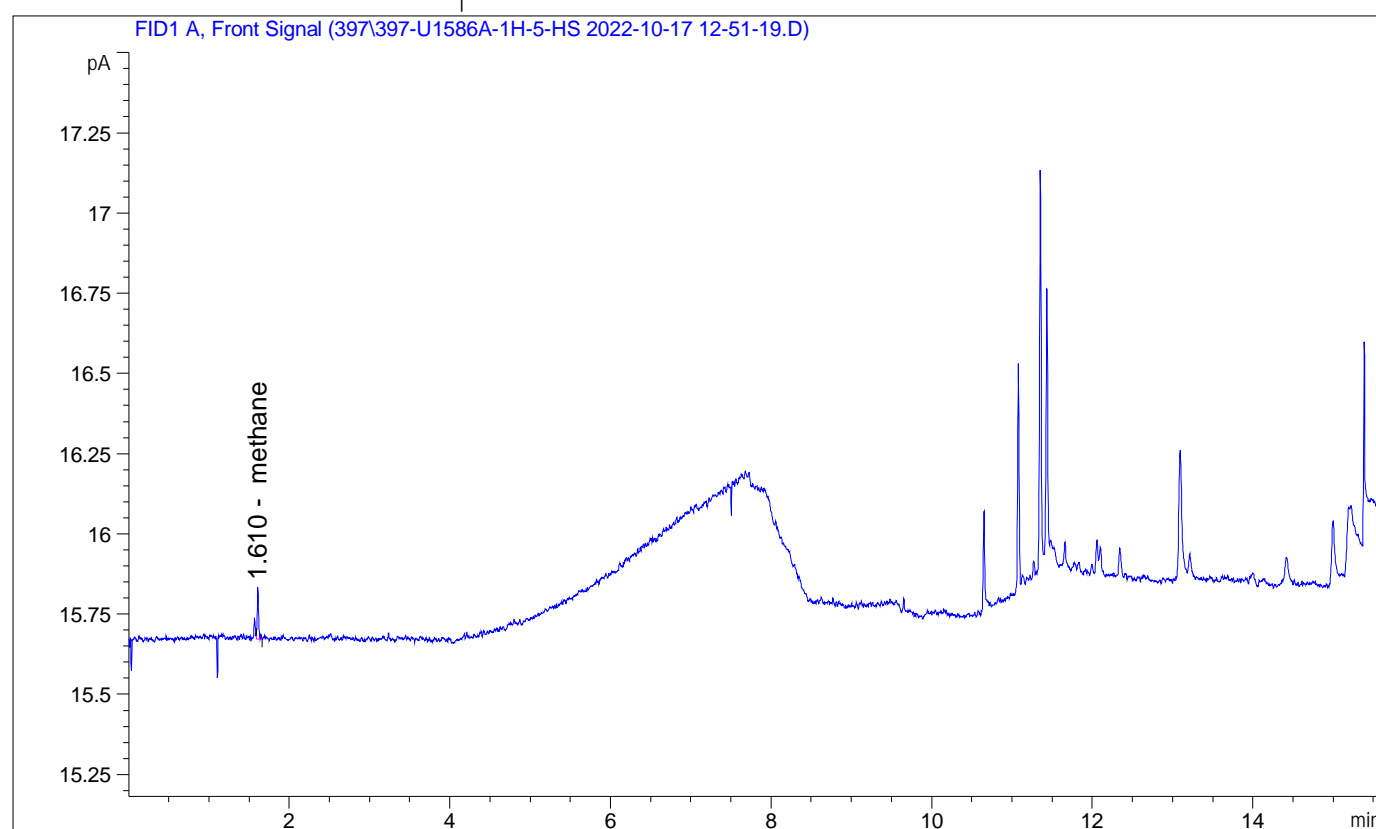

```
=====
External Standard Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :      10/14/2022 10:46:16 AM
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.610	VB	1.99761e-1	17.92346	3.58041		methane
1.982		-	-	-		ethane
2.709		-	-	-		ethene
3.967		-	-	-		propane
6.310		-	-	-		propene
6.662		-	-	-		i so-butane
6.894		-	-	-		n-butane
8.467		-	-	-		i so-pentane
8.621		-	-	-		n-pentane
9.818		-	-	-		i so-hexane
9.984		-	-	-		n-hexane

Totals : 3.58041

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Summed Peaks Report

Signal 1: FID1 A, Front Signal

Empty table.

Final Summed Peaks Report

Signal 1: FID1 A, Front Signal

Name	Total Area [pA*s]	Amount [ppm]
methane	1.99761e-1	3.5804
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 3.5804

Compound-related custom fields:

\*\*\* End of Report \*\*\*