Administrative Data

Institution   ABMC
Physicist   JP
PatientID   ANON0002
Patient Name   D, M
Comment   200 cGy/fx @ 100% IDL

Data Set A

M:\Eclipse Physics - Cancer Institute\ABMC\External Beam\Point Dose QA\RapidArc QA\2021\D, M\Composite.dcm

Data Set B

Added Data Sets:
A.mcc
B.mcc

Manipulations

Command	Data Set	Parameters	Value
Calibrate Air Density	B	kUser	1.040

Gamma 2D - Parameters

3.0 mm Distance- To- Agreement
3.0 % Dose difference with ref. to max. dose of selected slice
Use increased tolerance of 5.0 % dose diff. for values below 0.1 Gy (or AU)
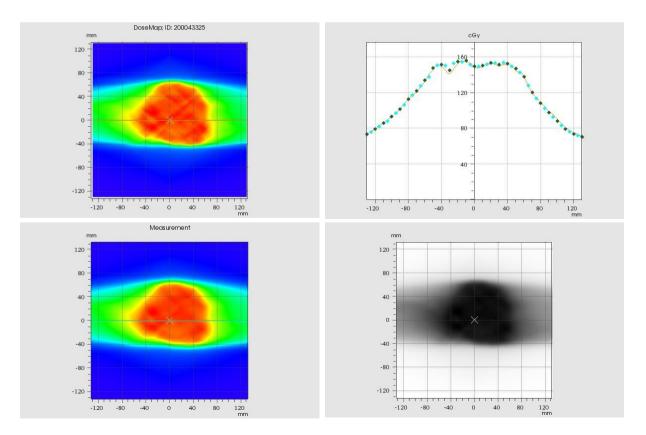Suppress dose below 5.0 % of max. dose of selected slice
Option "Use 2nd and 3rd pass" selected

Statistics

Number of Dose Points	1,405
Evaluated Dose Points	891 (63.4 %)
Passed	891 (100.0 %)
Failed	0 (0.0 %)
Result	100.0 % (Green)

Settings

Passing criteria	Gamma ≤ 1.0
Green	93.0 % to 100.0 %
Yellow	90.0 % to 93.0 %
Red	0.0 % to 90.0 %

DoseMap: ID: 200043325

Measurement