

Standard Name 31 of 118

↑

19106/170650D-A

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 29-Sep-23 Time: 15:34:49

Batch Name 4 of 4

↑

DKF19106 24050171IR-01 119055 EXP2400010

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal


Date: 13-Feb-24 Time: 11:01:19

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
DKF19106 24050171IR-01 119055 EXP2400010	D65 10 Deg	-0.43	0.01	0.70	-0.39	-0.62	-0.09	0.74		Warn	too dark	too dull	too green
DKF19106 24050171IR-01 119055 EXP2400010	F11 10 Deg	-0.36	0.14	0.81	-0.34	-0.68	0.01	0.76	0.16	Pass	too dark	too dull	too red

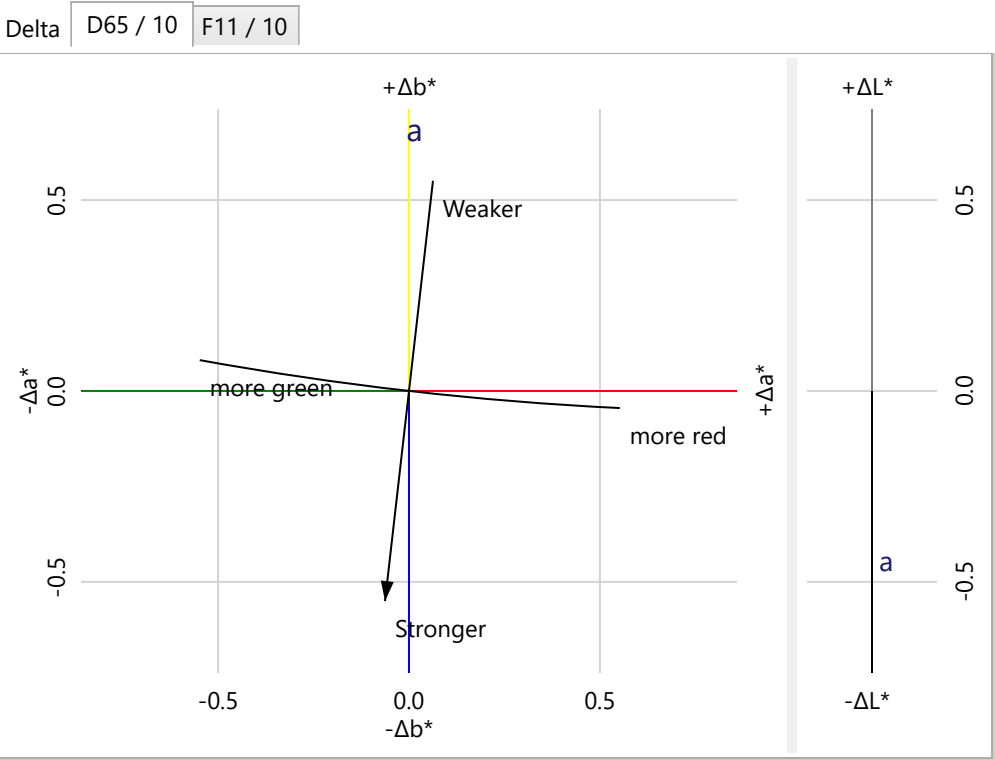

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form