

Standard Name 205 of 233

↑

20124/230920D-B

↓

Visual Hue Request:

New StdRetrieve StdStore StdList StdUpdate Std

Instrument Setup:%R LAV SCI UV Cal

Date: 04-Apr-24Time: 21:34:14

Batch Name 1 of 2

↑

HJY20124 5506649 136348 DOM2400492

↓

New BatRetrieve BatStore BatList BatUpdate Bat

Instrument Setup: %R LAV SCI UV Cal


Date: 17-Apr-24Time: 09:18:19

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: ( 2.00 1.00)

Measured by:

<u>Batch Name</u>				<u>III/Obs</u>	<u>DL*</u>	<u>Da*</u>	<u>Db*</u>	<u>DL*/ISL</u>	<u>DC*/cSC</u>	<u>DH*/SH</u>	<u>CMC DE</u>	<u>M.I.</u>	<u>P/E</u>	<u>Color</u>	<u>Comments</u>
HJY20124	5506649	136348	DOM2400492	D65 10 Deg	1.17	-0.79	0.22	0.58	0.23	-0.40	<b>0.74</b>		Pass	too light	too bright too yellow
HJY20124	5506649	136348	DOM2400492	F11 10 Deg	1.23	-1.04	0.28	0.64	0.22	-0.60	<b>0.91</b>	0.41	Pass	too light	too bright too yellow

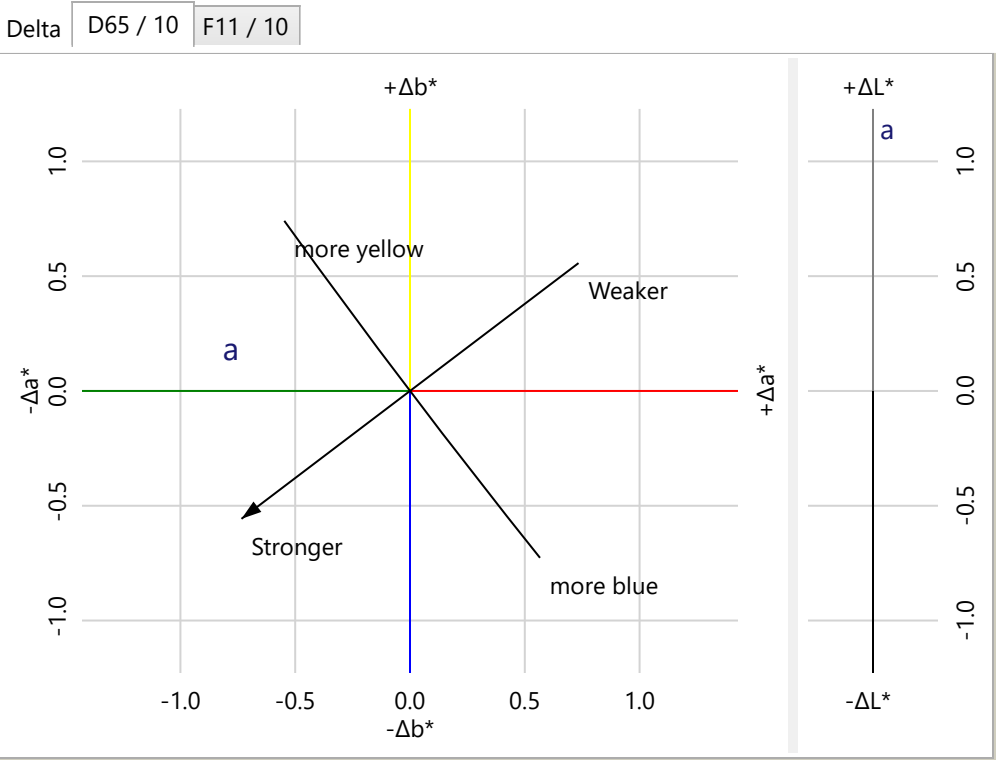

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form