


# UUT Report

**Station ID:** IT-W-7303101  
**Serial Number:** NONE  
**Date:** giovedì 19 gennaio 2023  
**Time:** 11:22:45  
**Operator:** ITLAVIT1  
**Execution Time:** 00:29:41.006  
**Number of Results:** 831  
**UUT Result:** Passed

---

**Begin Sequence: MainSequence**  
(C:\Users\itlavit1\OneDrive - ABB\LabRnD\_Shared\TestStand\Sequences\Accuracy\D13\D13 - Zera - Accuracy.seq)

DUT recap	
Status:	Done
TestResults/Data:	
Type Designator:	B3D4MB111A
FW Version:	0.11.1
Serial Number:	"
Switch on Zera	
Status:	Passed
Module Time:	14.529

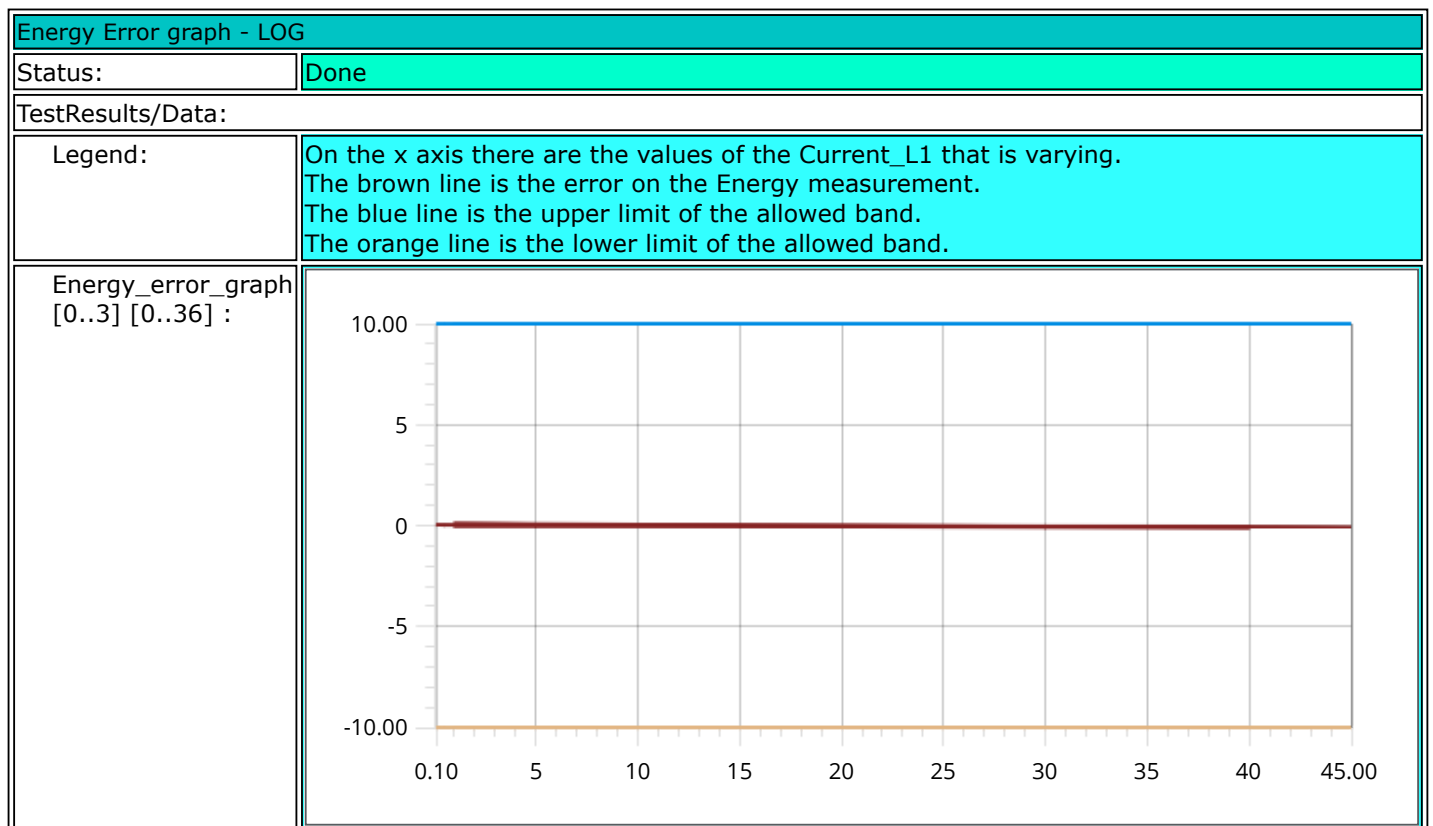

Switch off Zera	
Status:	Passed
Module Time:	11.4996

**End Sequence: MainSequence**

