

UUT Report

Station ID: IT-W-7303101
Serial Number: NONE
Date: martedì 14 marzo 2023
Time: 13:48:45
Operator: ITLAVIT1
Execution Time: 00:07:51.058
Number of Results: 400
UUT Result: Terminated


Begin Sequence: MainSequence
(C:\Users\itlavit1\OneDrive - ABB\LabRnD_Shared\TestStand\Sequences\EQ Meter\Power Fail\D13\D13 - Omicron - Repeated Power Fail.seq)

DUT recap	
Status:	Done
TestResults/Data:	
Type Designator:	B3D4MB111A
FW Version:	0.13.2
Serial Number:	"

Total Active Import	
Status:	Passed
Numeric:	14
Limits:	
Low:	13.8875
High:	15.6125
Comparison Type:	GELE(>= <=)
Total Active Import	
Status:	Failed
Total Active Import	
Status:	Passed
Numeric:	20
Limits:	
Low:	19.8875
High:	21.6125
Comparison Type:	GELE(>= <=)
Total Active Import	
Status:	Passed
Total Active Import	
Status:	Passed
Numeric:	26
Limits:	
Low:	24.8875
High:	26.6125
Comparison Type:	GELE(>= <=)
Total Active Import	

[illegible]


Energy Save During	
Status:	Passed
Energy Save	
Status:	Failed
Energy Save During	
Status:	Passed
Energy Save	
Status:	Failed
Energy Save During	
Status:	Passed

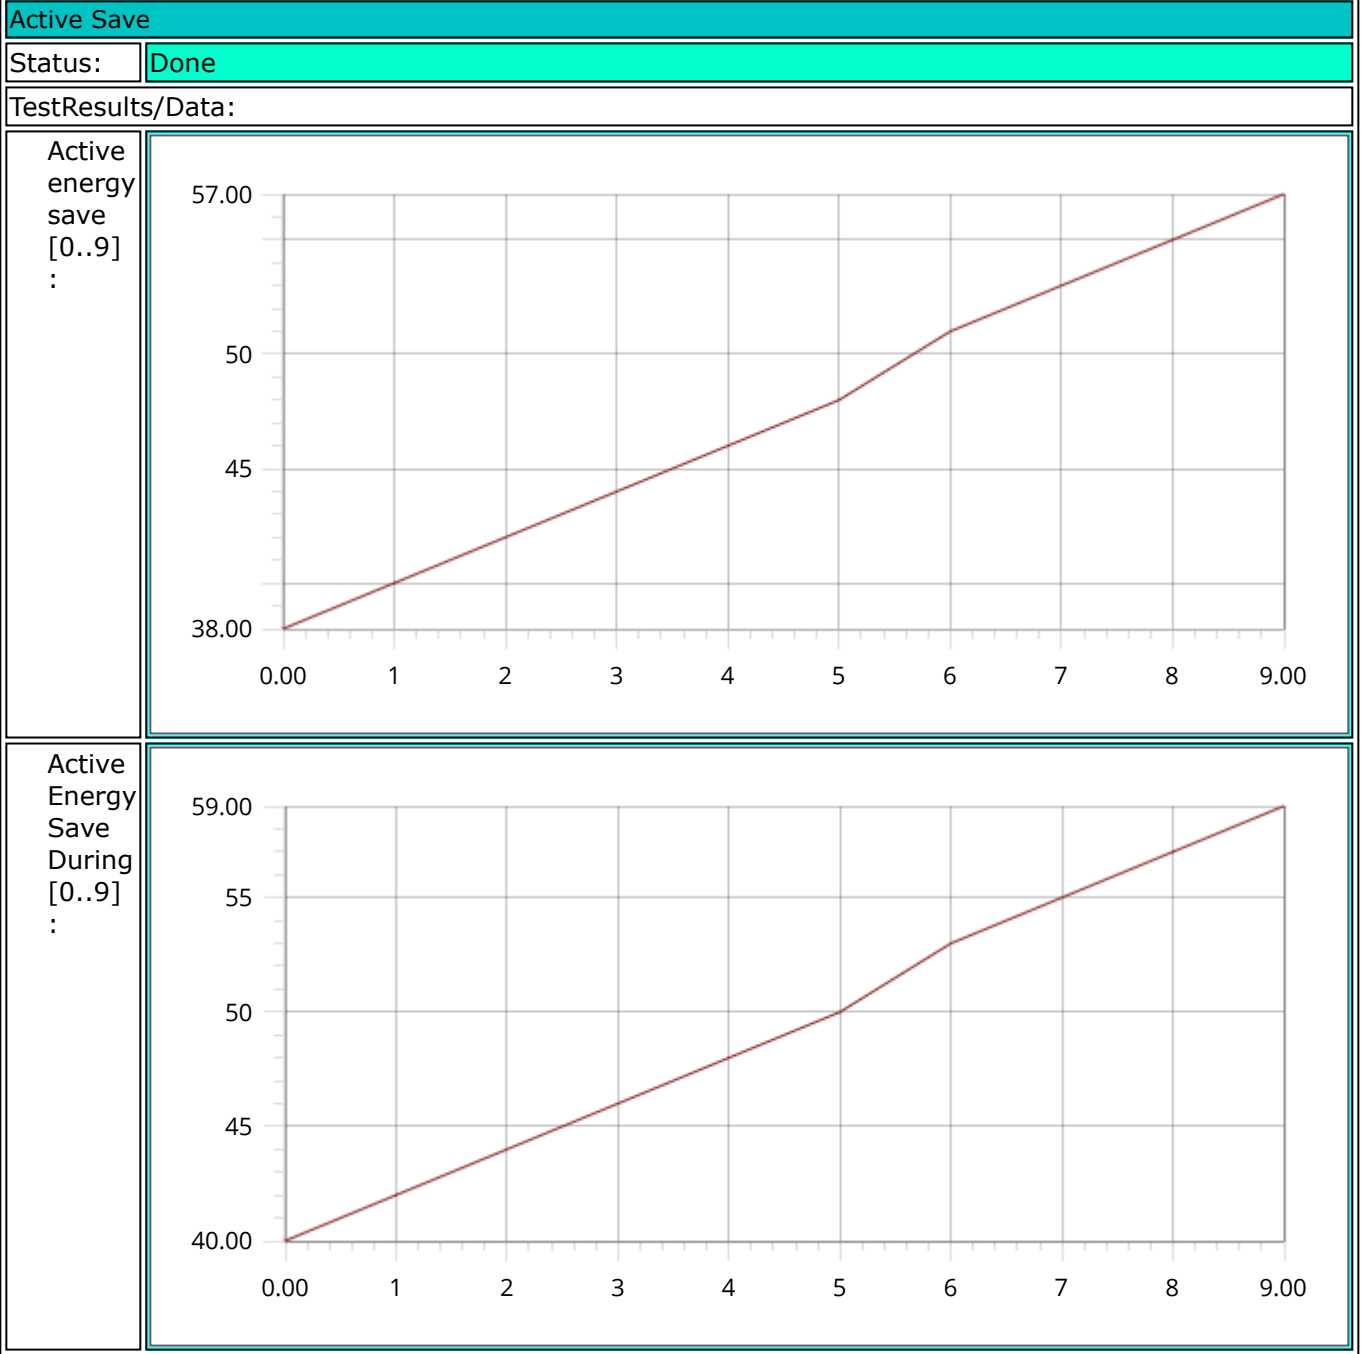

Energy Flash	
Status:	Passed
Numeric:	59
Limits:	
Low:	62
Comparison Type:	LT(<)

Energy Flash	
Status:	Passed
Numeric:	62
Limits:	
Low:	65
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	65
Limits:	
Low:	69
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	69
Limits:	
Low:	72
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	72
Limits:	
Low:	75
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	75
Limits:	
Low:	78
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	78
Limits:	
Low:	82
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	82
Limits:	
Low:	85
Comparison Type:	LT(<)
Energy Flash	
Status:	Passed
Numeric:	85
Limits:	
Low:	88
Comparison Type:	LT(<)

Energy Flash	
Status:	Passed
Numeric:	88
Limits:	
Low:	92
Comparison Type:	LT(<)



End Sequence: MainSequence

End UUT Report

