UUT Report

Station ID:	**IT-W-7303101**
Serial Number:	**NONE**
Date:	**mercoledì 7 giugno 2023**
Time:	**09:17:08**
Operator:	**administrator**
Execution Time:	**1548.9223386 seconds**
Number of Results:	**19262**
UUT Result:	**Passed**
Serial Number:	**4294967295**
Type Designator:	**B1-D3BB-111A**
FW Version:	**0.16.1**
Power Supply:	**Zera**

Begin Sequence: MainSequence
(C:\Users\itlavit1\OneDrive - ABB\LabRnD_Shared\TestStand\Sequences\EQ Meter\New Sequences\Realtime_sampling.seq)

DUT info	
Status:	Done
Serial Number:	4294967295
Type Designator:	B1-D3BB-111A
FW Version:	0.16.1

Test Point	
Status:	Done
Current:	0.25
Power Factor:	1

Voltage - LOG	
Status:	Done
Accuracy[0..1] [0..599]:	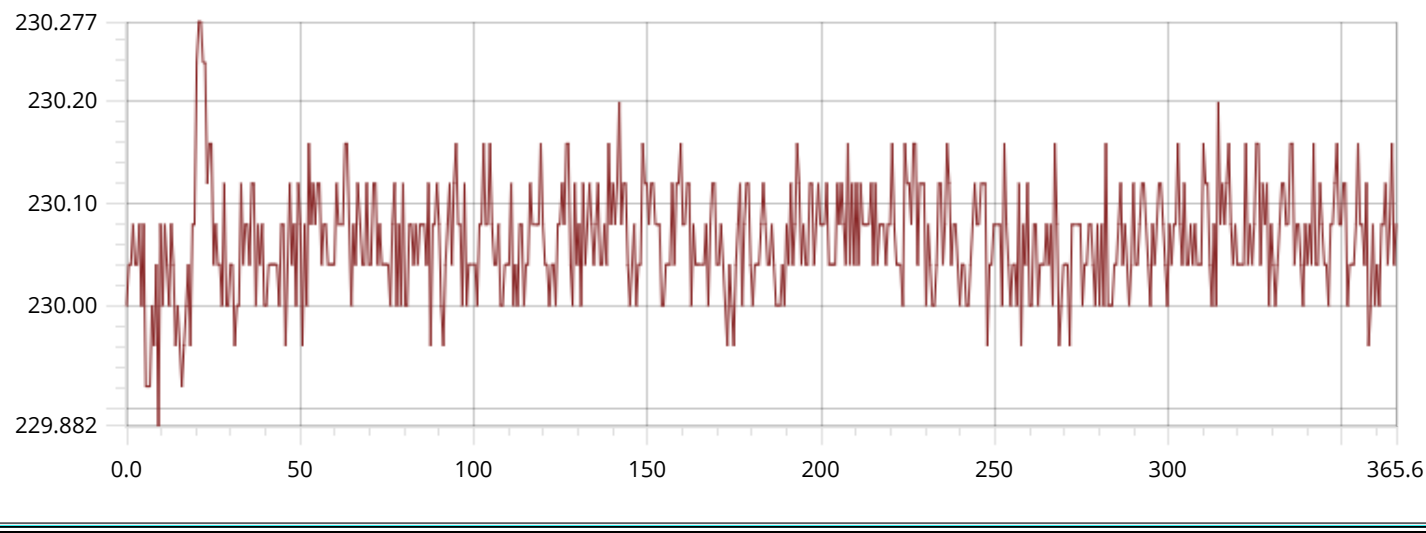

Current - LOG	
Status:	Done
Accuracy[0..1] [0..599]:	

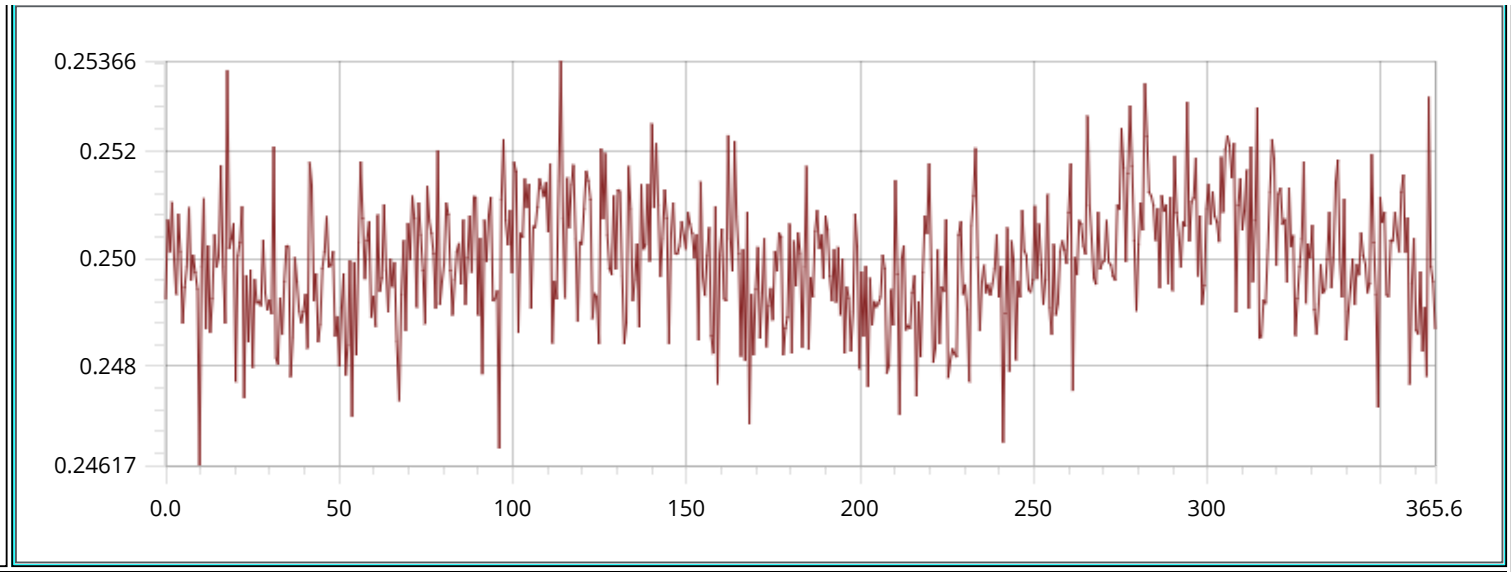

Active power - LOG

Status:	Done

Accuracy[0..1] [0..599]:

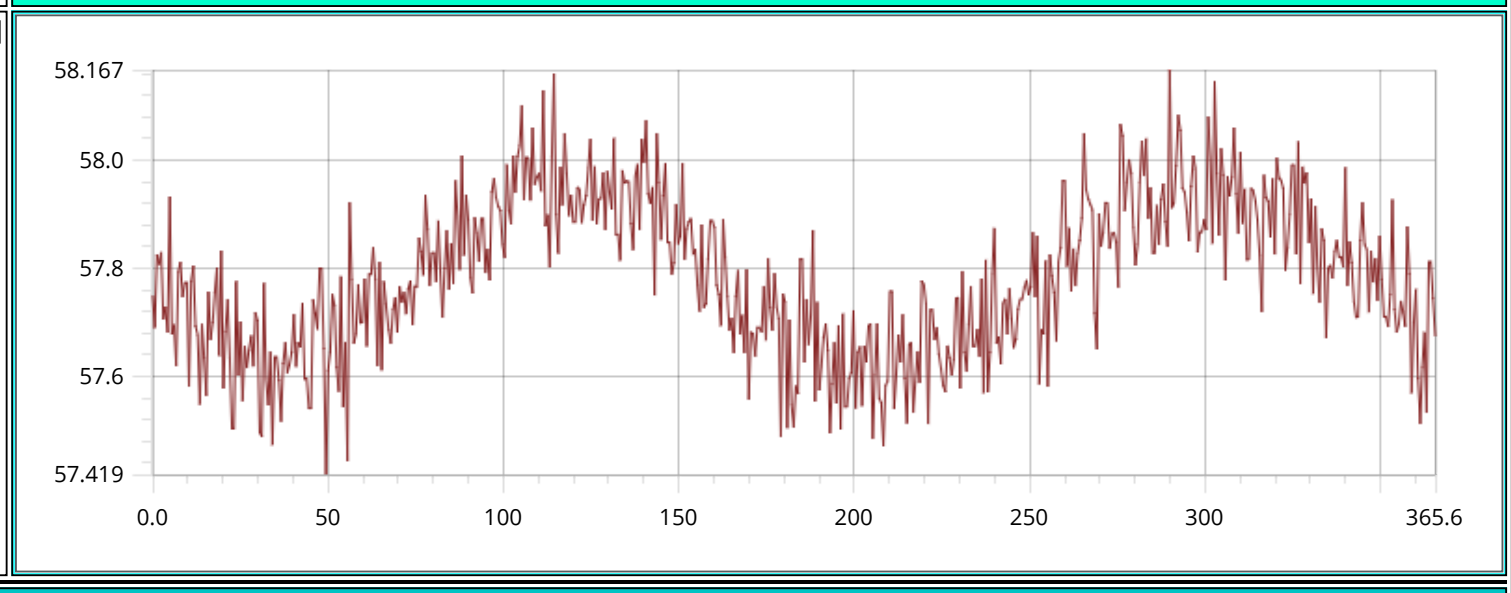

Test Point

Status:	Done
Current:	1
Power Factor:	1

Voltage - LOG

Status:	Done

Accuracy[0..1] [0..599]:

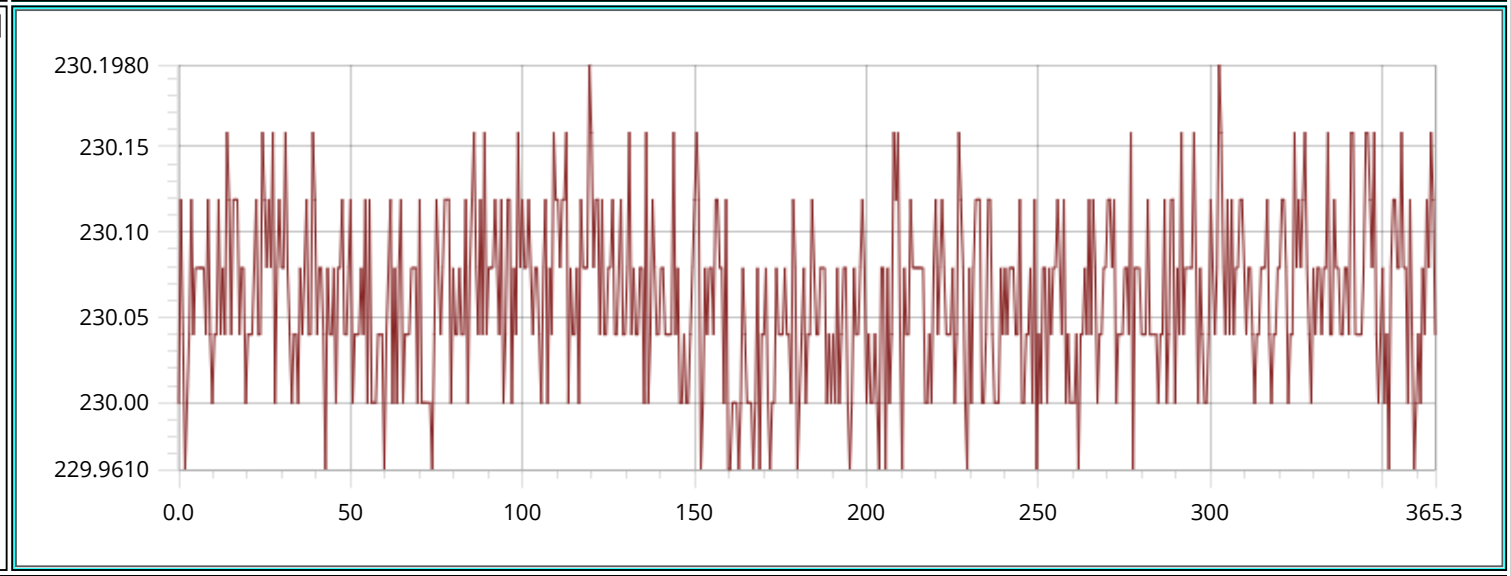

Current - LOG

Status:	Done
Accuracy[0..1] [0..599]:	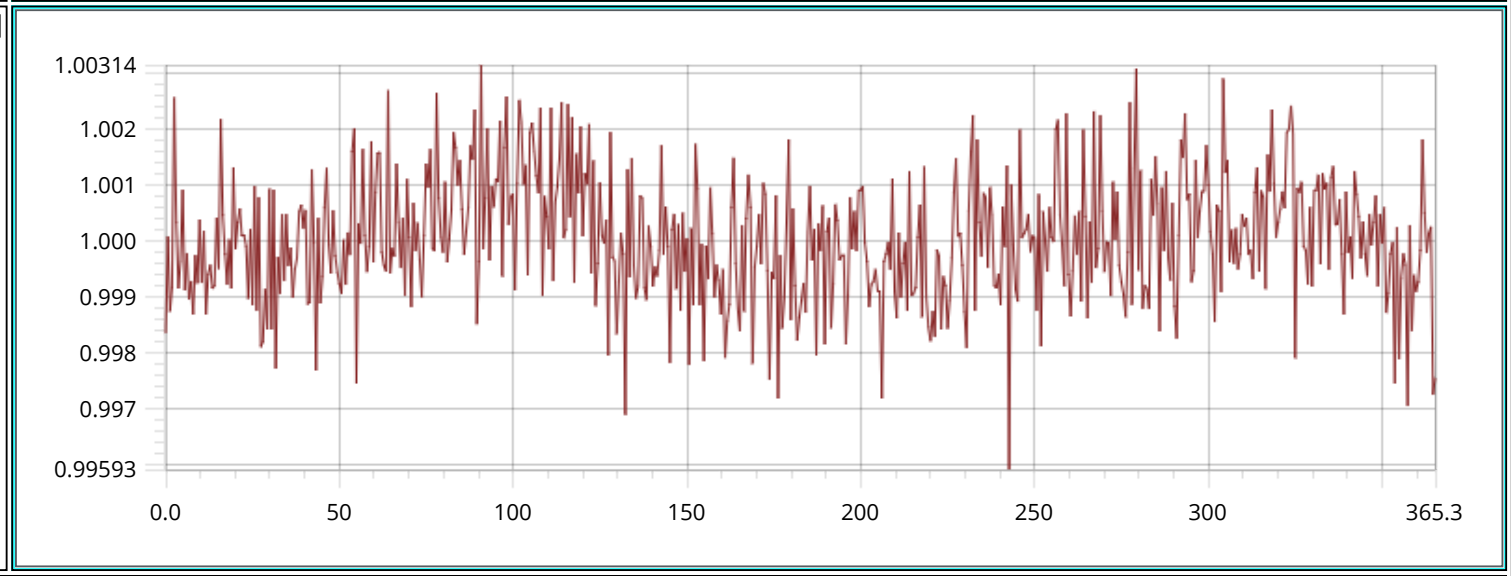

Active power - LOG

Status:	Done
Accuracy[0..1] [0..599]:	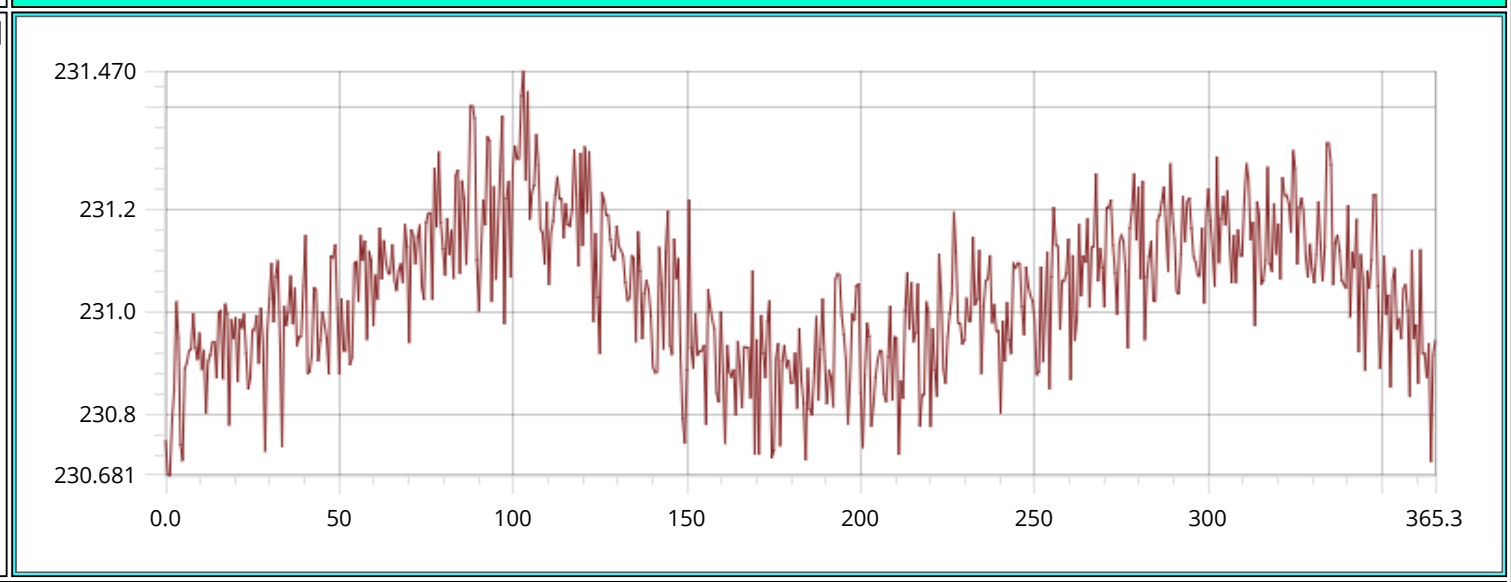

Test Point

Status:	Done
Current:	1
Power Factor:	0.5

Voltage - LOG

Status:	Done
Accuracy[0..1] [0..599]:	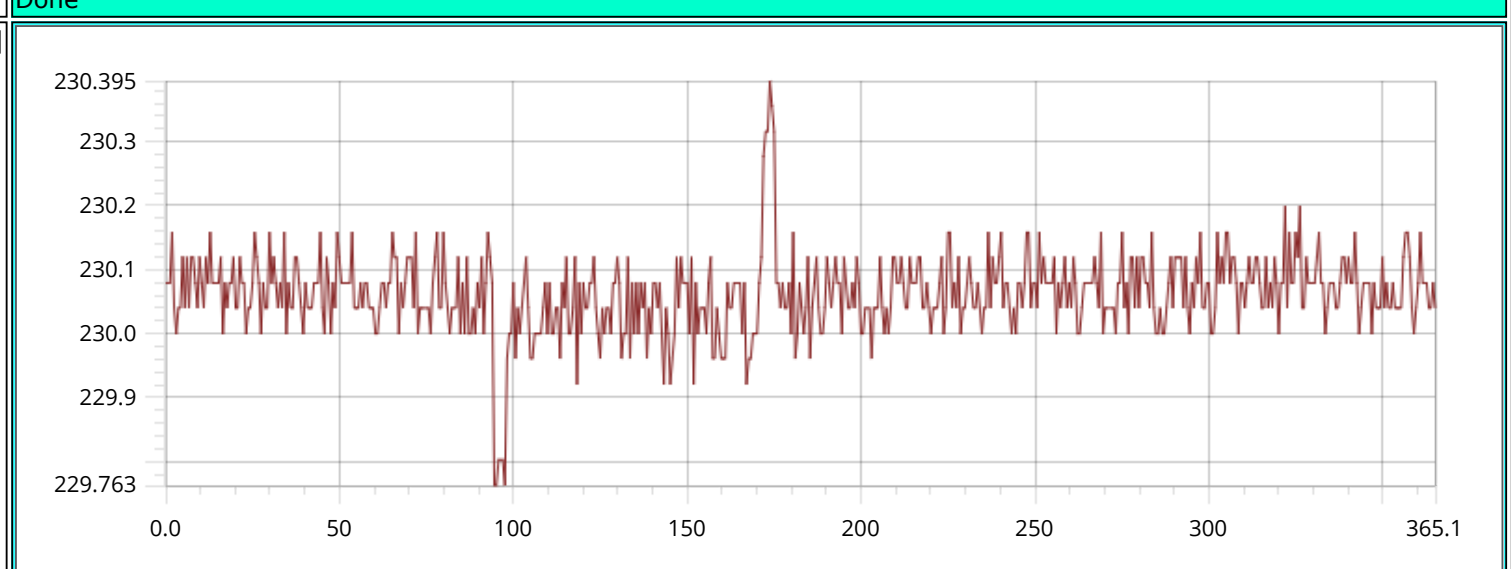

Current - LOG

Status:	Done
Accuracy[0..1] [0..599]:	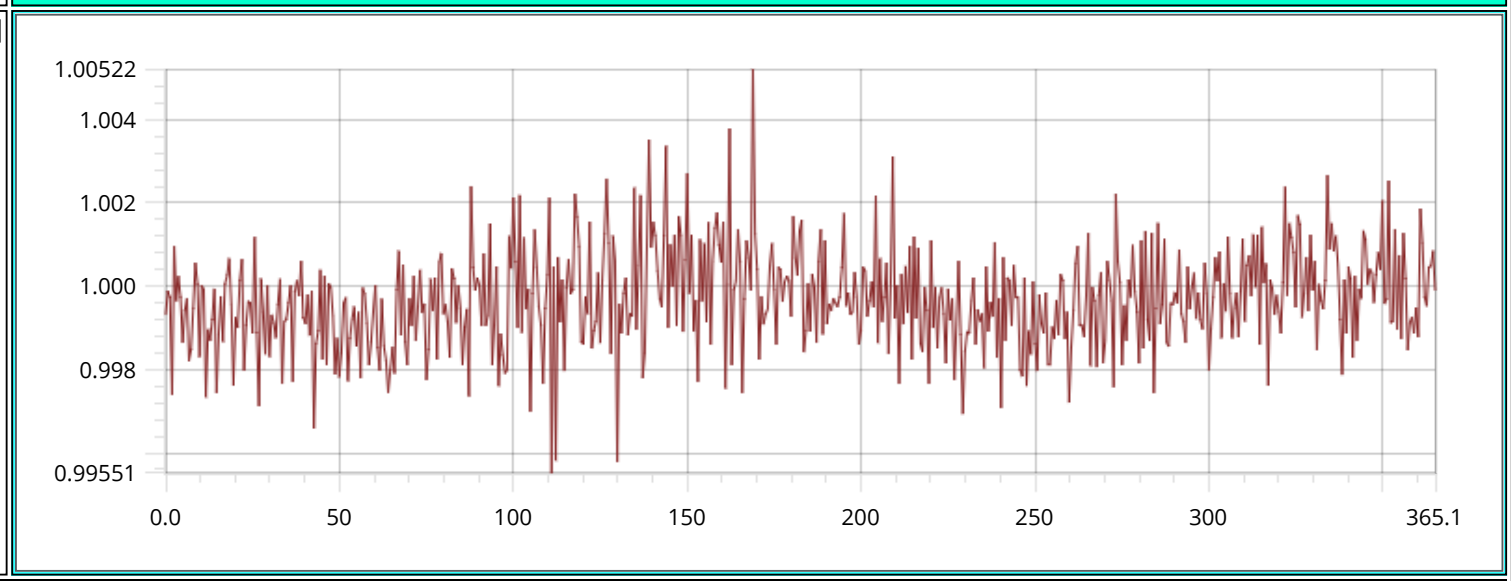

Active power - LOG

Status:	Done
Accuracy[0..1] [0..599]:	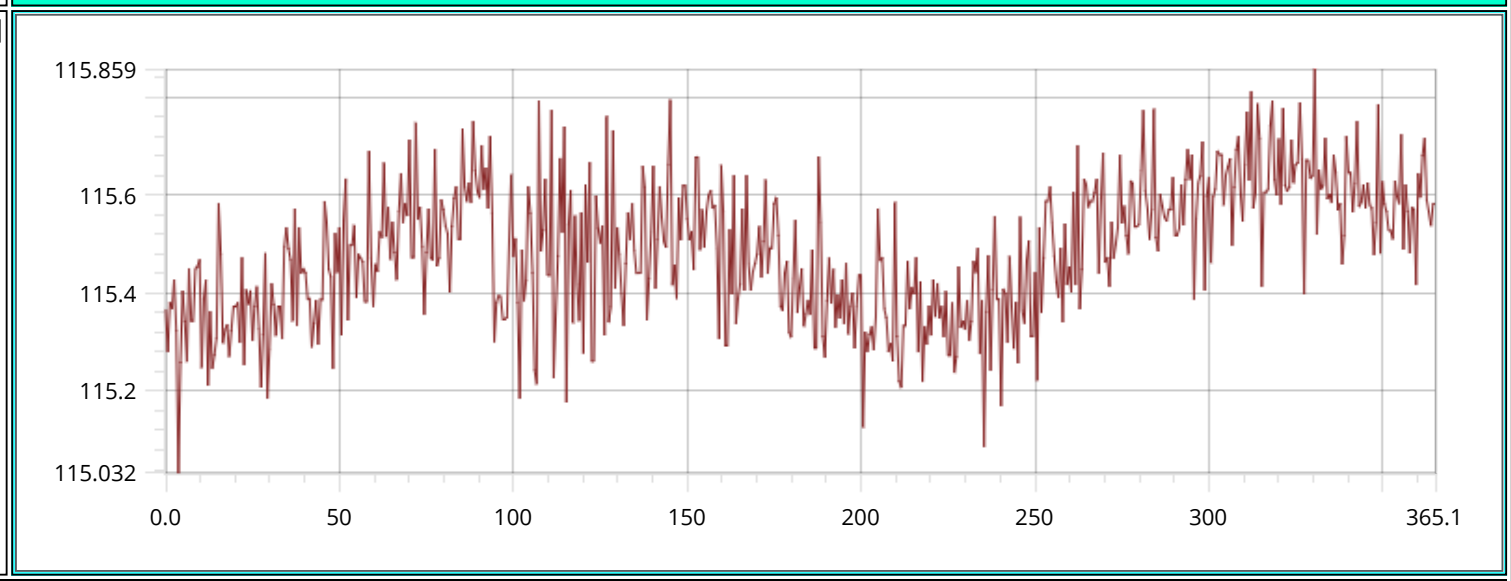

Test Point

Status:	Done
Current:	1
Power Factor:	0.7986355100473

Voltage - LOG

Status:	Done
Accuracy[0..1] [0..599]:	

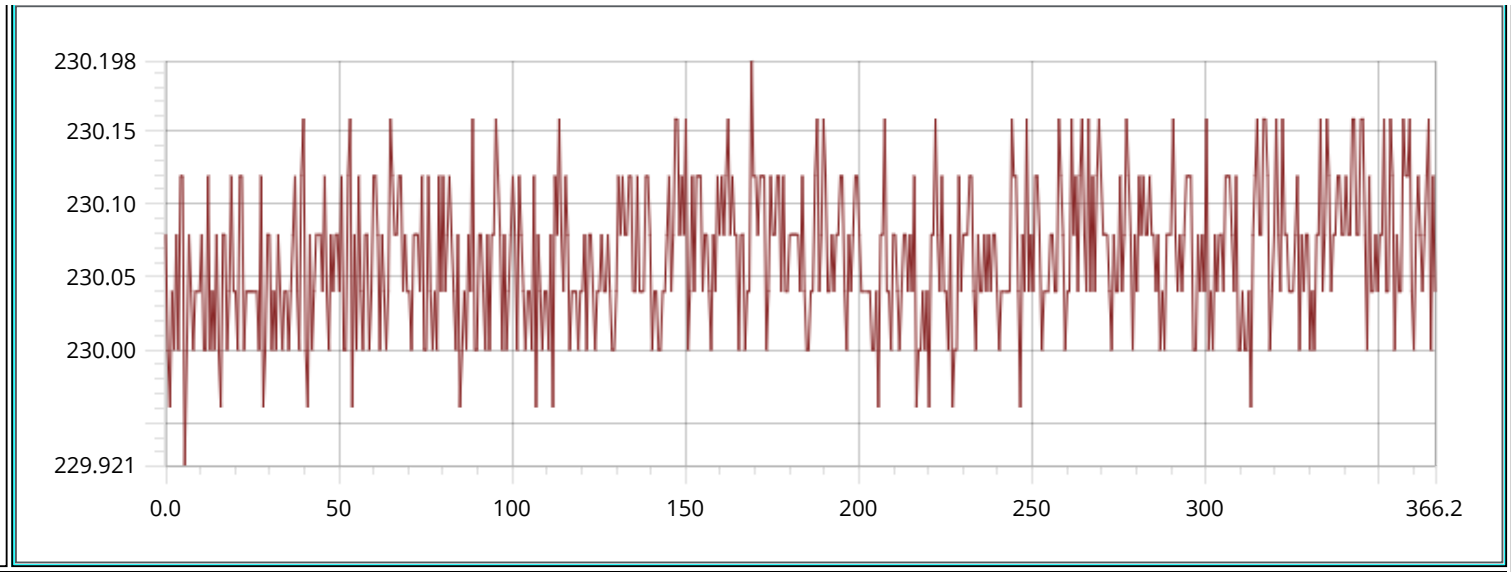

Current - LOG	
Status:	Done
Accuracy[0..1] [0..599]:	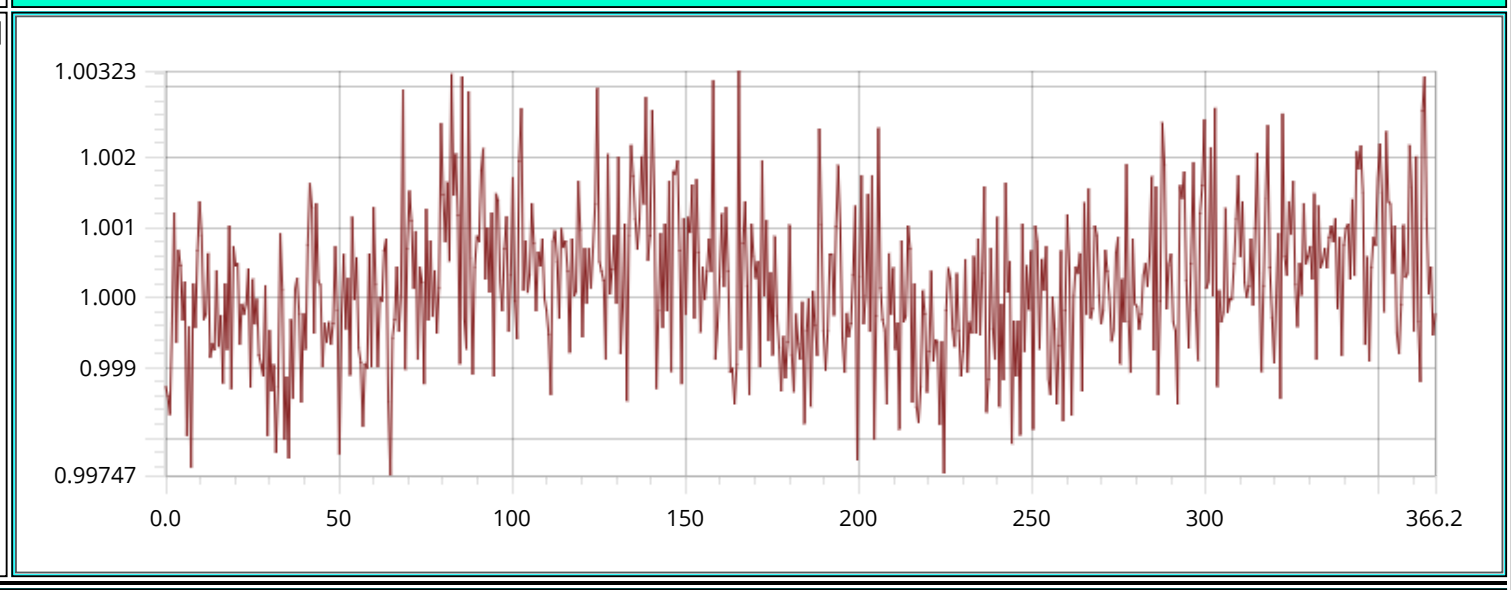

Active power - LOG	
Status:	Done
Accuracy[0..1] [0..599]:	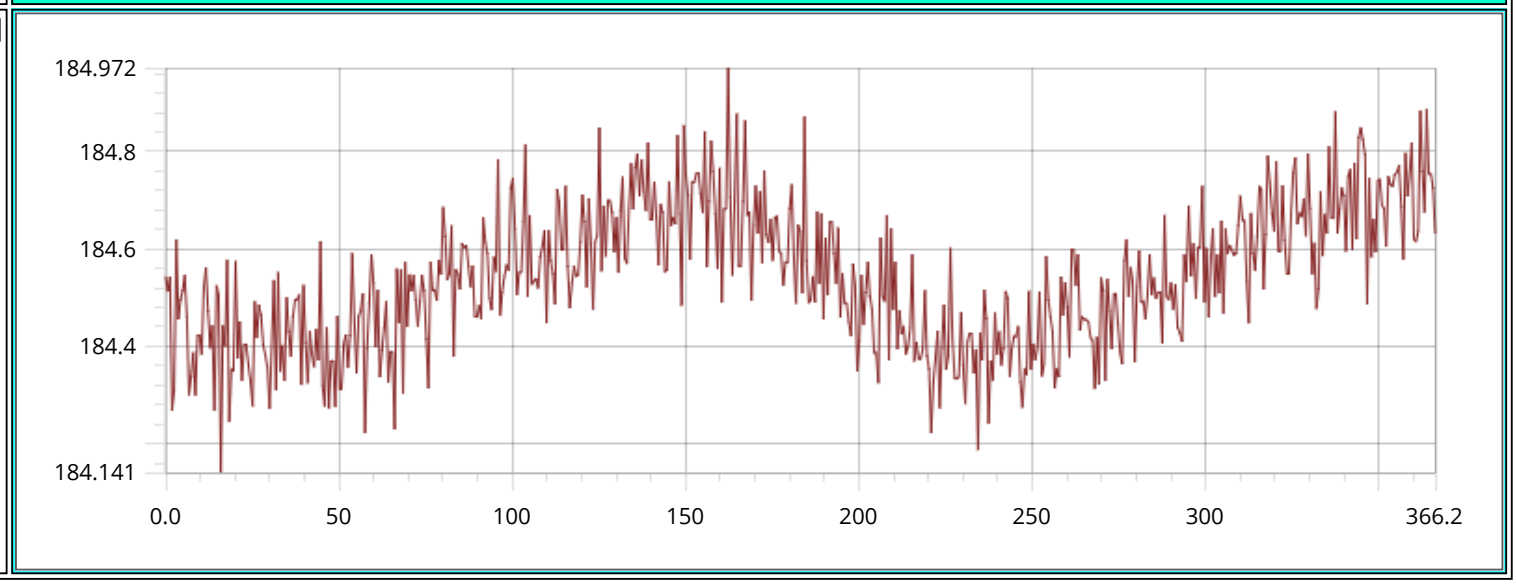

End Sequence: MainSequence

End UUT Report