

UUT Report

Station ID:

Serial Number:

Date:

Time:

Operator:

Execution Time:

Number of Results:

UUT Result:

Serial Number:

Type Designator:

FW Version:

Power Supply:

IT-W-7303101

NONE

giovedì 29 giugno 2023

12:06:54

administrator

1767.4688552 seconds

565

Passed

4294967295


B3-D4MB-111A

0.17.0

Zera

Begin Sequence: MainSequence

(C:\Users\itlavit1\OneDrive - ABB\LabRnD_Shared\TestStand\Sequences\EQ Meter\New Sequences\Energy Accuracy.seq)

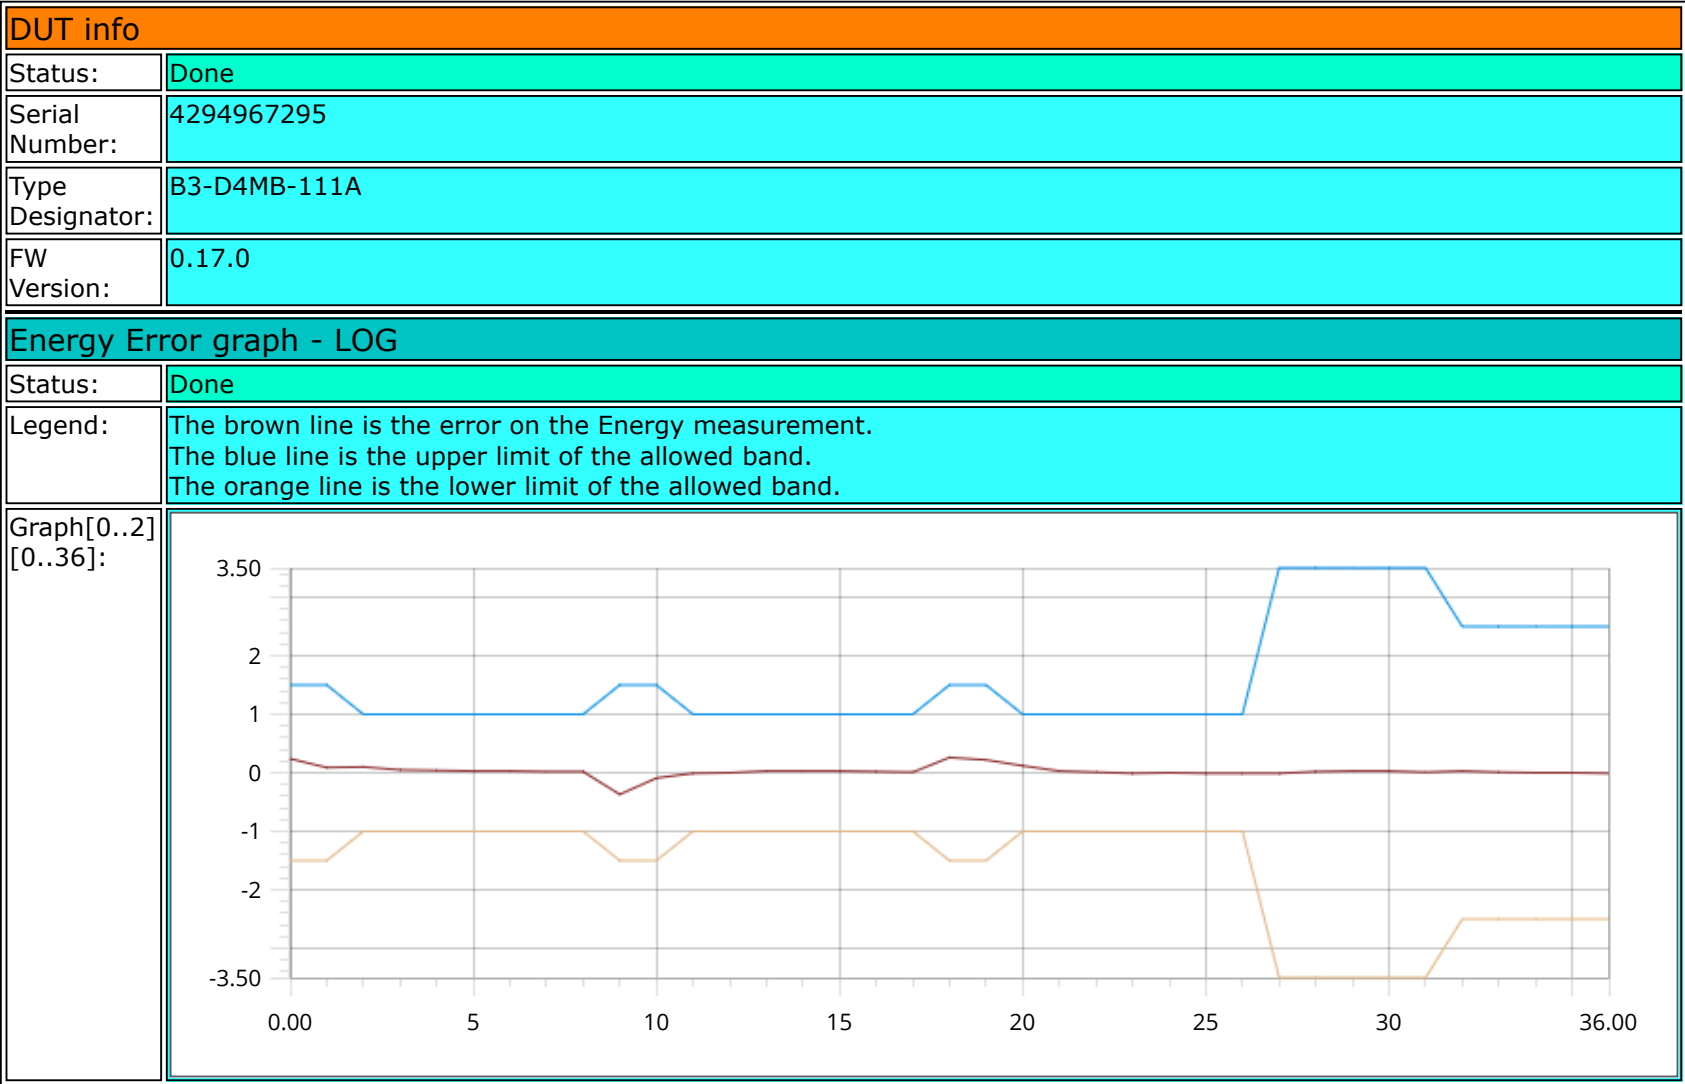

End Sequence: MainSequence

End UUT Report
