

Urogenital microbiome composition test


Androbiome Screen

Logotype

Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: Sample_1

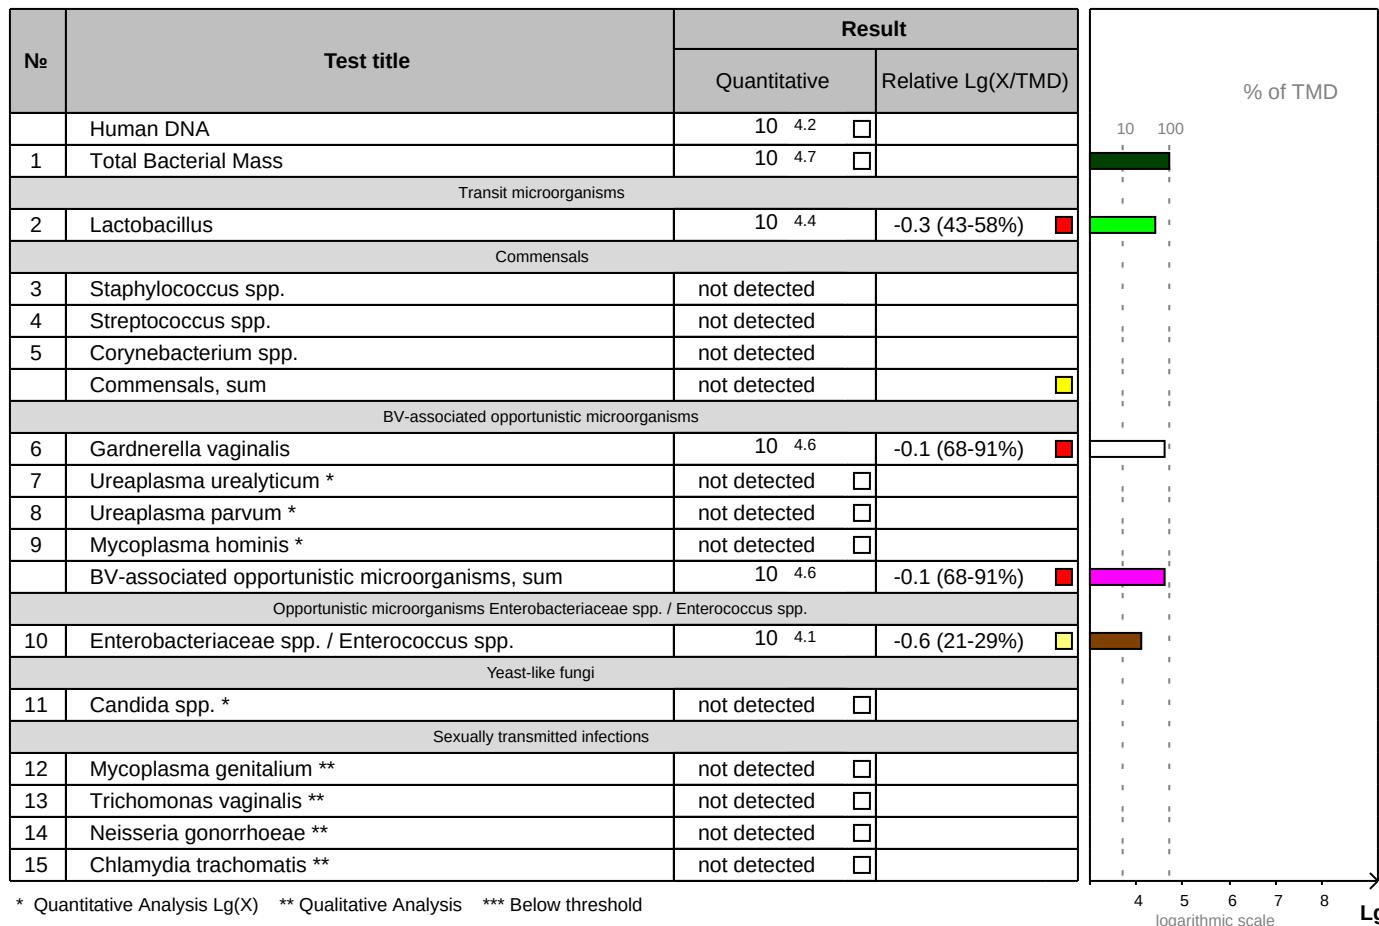

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. DNA is not detected.

Exceeding the threshold values of transient microflora does not allow to make a correct conclusion about the real composition of the bacterial microbiome be long to patient. microflora e.g. BV-associated bacteria, can be the cause of acute inflammation of the lower parts of the urogenital tract. The result of the study directly depends on compliance with the rules of preparation for the collection of biomaterial.

Study was carried out by

Date
Signature

Urogenital microbiome composition test

Androbiome Screen




Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: Sample_2

№	Test title	Result	
		Quantitative	Relative Lg(X/TMD)
	Human DNA	10 4.4	☐
1	Total Bacterial Mass	10 3.2	☐
Transit microorganisms			
2	Lactobacillus	not detected	☐
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	not detected	
	Commensals, sum	not detected	☐
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	☐
7	Ureaplasma urealyticum *	not detected	☐
8	Ureaplasma parvum *	not detected	☐
9	Mycoplasma hominis *	not detected	☐
	BV-associated opportunistic microorganisms, sum	not detected	☐
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	not detected	☐
Yeast-like fungi			
11	Candida spp. *	below TH ***	☐
Sexually transmitted infections			
12	Mycoplasma genitalium **	not detected	☐
13	Trichomonas vaginalis **	not detected	☐
14	Neisseria gonorrhoeae **	not detected	☐
15	Chlamydia trachomatis **	not detected	☐

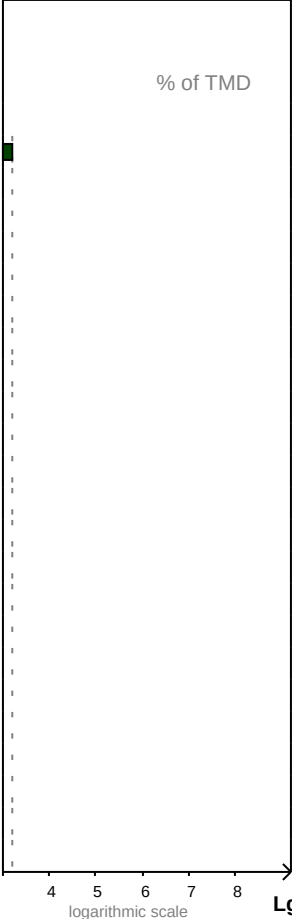

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:
STIs DNA is not detected.
Candida spp. below threshold.
The bacterial microbiome composition is normal.

Study was carried out by

Date
Signature

Urogenital microbiome composition test


Androbiome Screen



Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: Sample_3

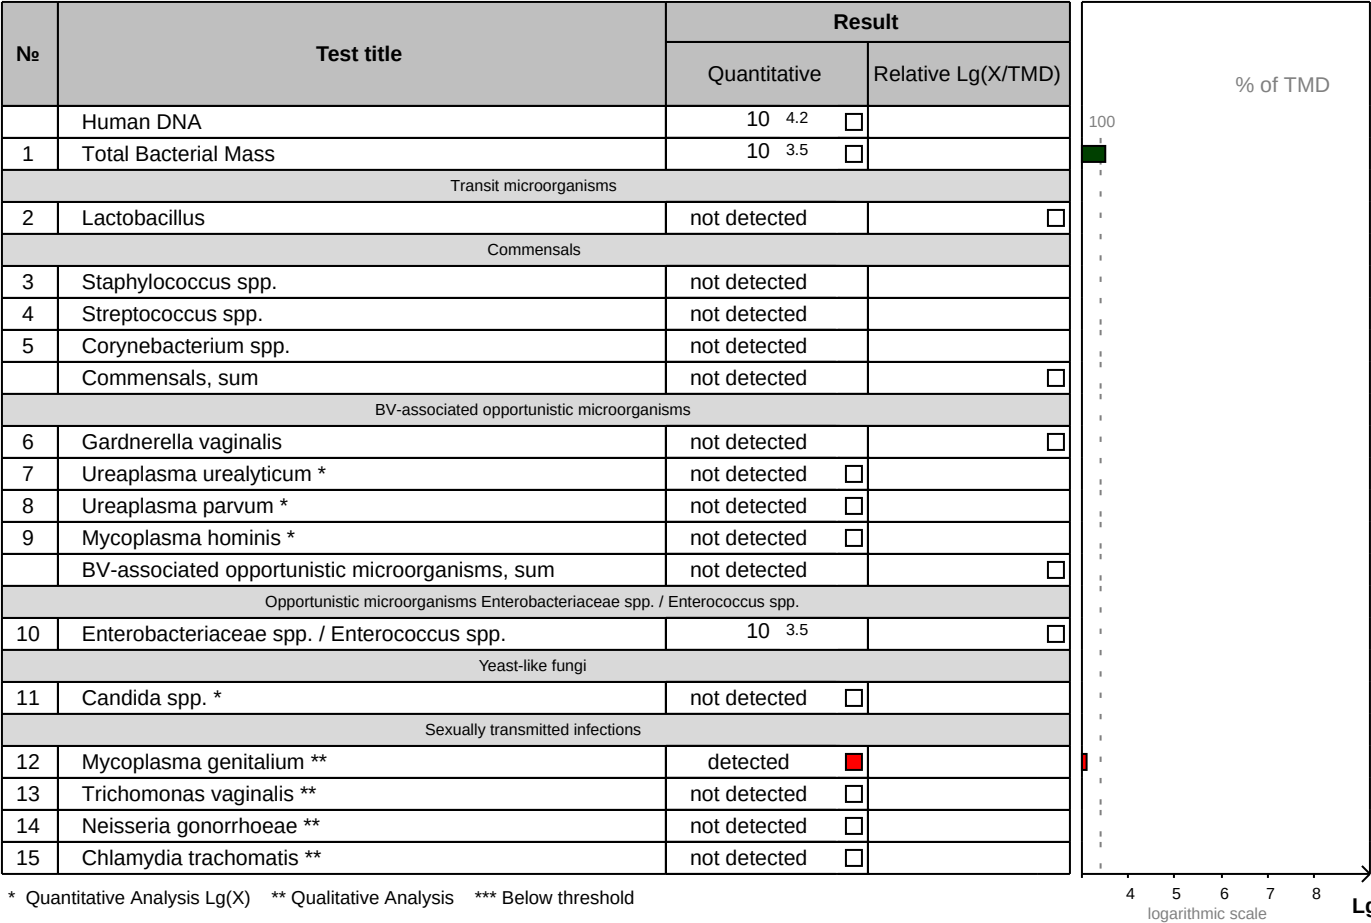

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:
DETECTED: Mycoplasma genitalium.
Candida spp. DNA is not detected.
The bacterial microbiome composition is abnormal: STIs DNA is detected, the balance between the components of normal flora is not changed.

Study was carried out by

Date
Signature

Urogenital microbiome composition test


Androbiome Screen

Logotype

Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: Sample_4

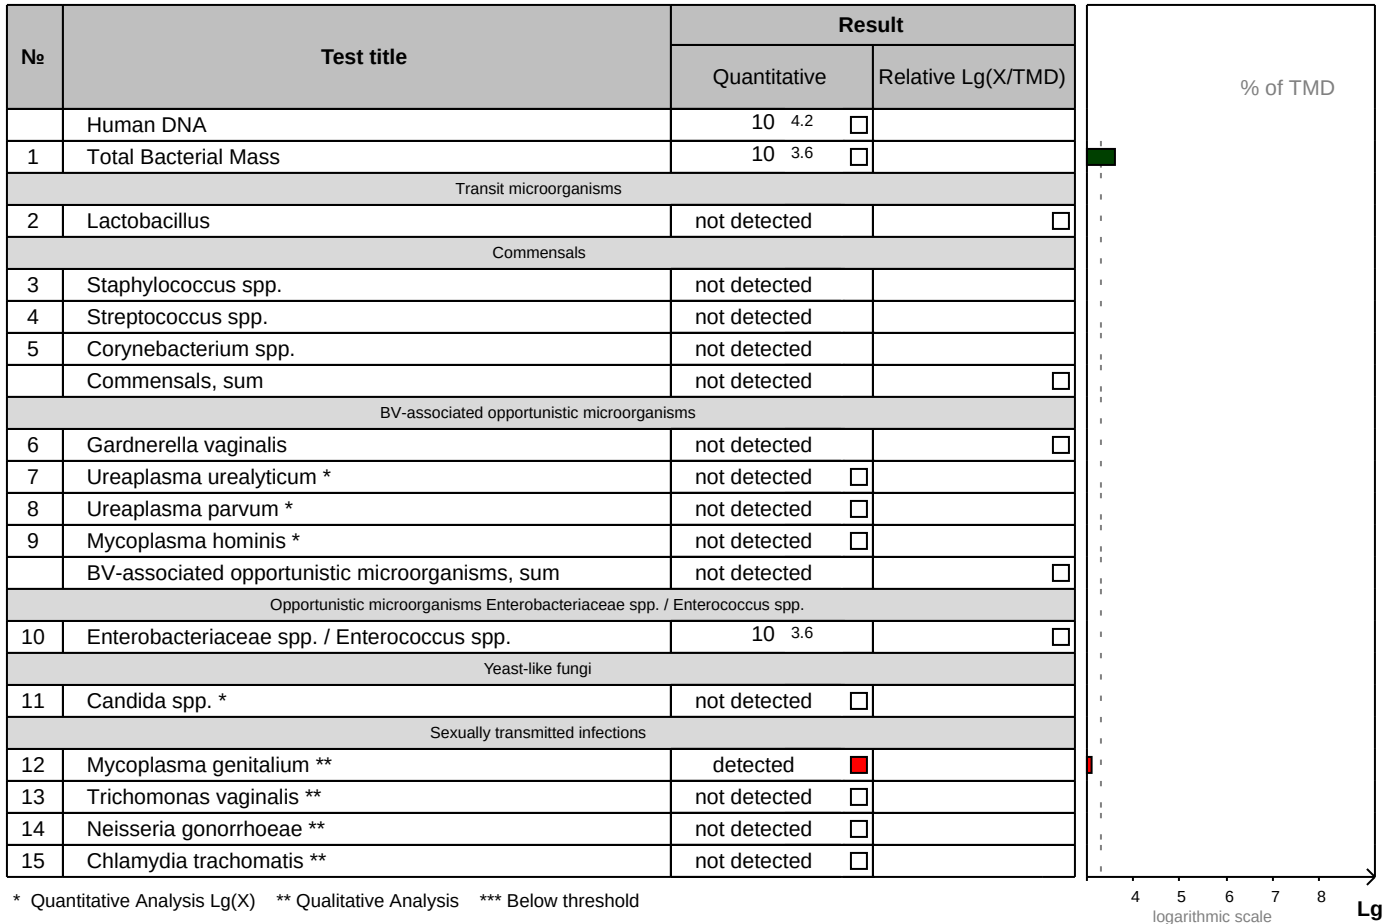

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

DETECTED: Mycoplasma genitalium.

Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: STIs DNA is detected, the balance between the components of normal flora is not changed.

Study was carried out by

Date
Signature

Urogenital microbiome composition test


Androbiome Screen

Logotype

Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: Sample_5

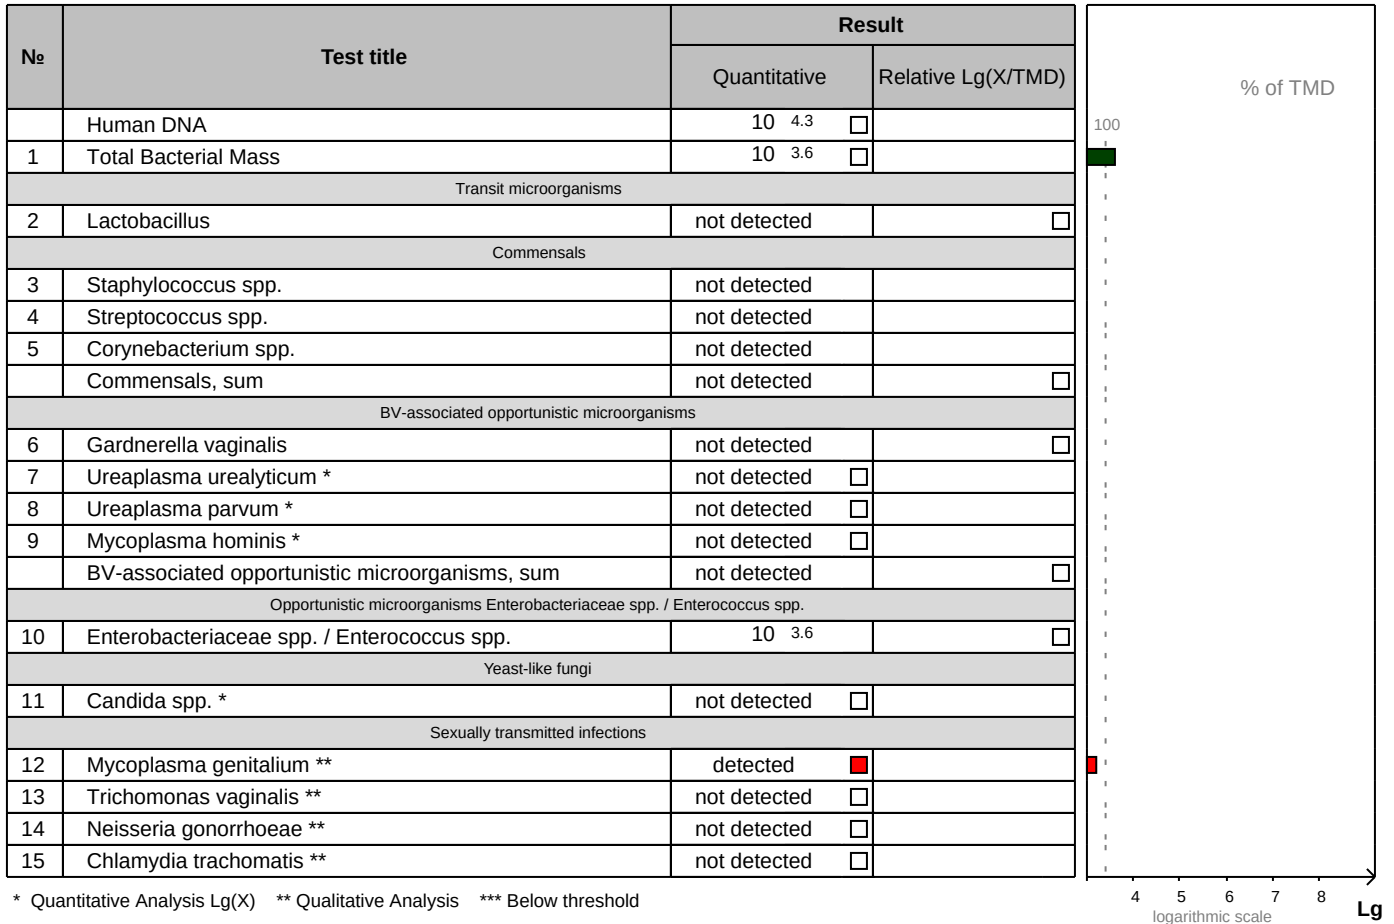

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

DETECTED: Mycoplasma genitalium.

Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: STIs DNA is detected, the balance between the components of normal flora is not changed.

Study was carried out by

Date
Signature

Urogenital microbiome composition test

Androbiome Screen


Logotype

Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: Sample_6

№	Test title	Result	
		Quantitative	Relative Lg(X/TMD)
	Human DNA	10 4.2	☐
1	Total Bacterial Mass	10 3.5	☐
Transit microorganisms			
2	Lactobacillus	not detected	☐
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	not detected	
	Commensals, sum	not detected	☐
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	☐
7	Ureaplasma urealyticum *	not detected	☐
8	Ureaplasma parvum *	not detected	☐
9	Mycoplasma hominis *	not detected	☐
	BV-associated opportunistic microorganisms, sum	not detected	☐
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	10 3.5	☐
Yeast-like fungi			
11	Candida spp. *	not detected	☐
Sexually transmitted infections			
12	Mycoplasma genitalium **	detected	☒
13	Trichomonas vaginalis **	not detected	☐
14	Neisseria gonorrhoeae **	not detected	☐
15	Chlamydia trachomatis **	not detected	☐

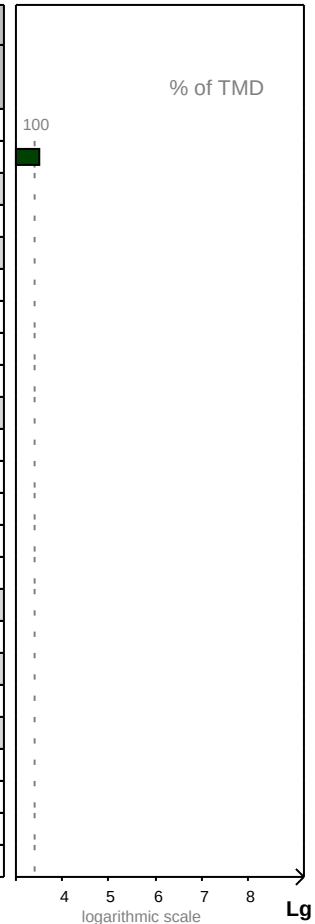

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

DETECTED: Mycoplasma genitalium.

Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: STIs DNA is detected, the balance between the components of normal flora is not changed.

Study was carried out by

Date
Signature